

# **Epsilon 1-4 LSCplus**

Part no. 111141

# **Epsilon 2-4 LSCplus**

Part no. 111144





# **Operating Manual**

Read the manual thoroughly before use and retain it for later use!






In case of inquiries, please state the following numbers:
Order number:

Serial number:

© Copyright by Martin Christ Gefriertrocknungsanlagen GmbH An der Unteren Söse 50 37520 Osterode am Harz Germany

Tel.: +49 (0) 5522 / 5007-0 Fax: +49 (0) 5522 / 5007-12 Web: www.martinchrist.de E-mail: info@martinchrist.de







1	G	ener	al information	9
	1.1	Imp	ortance of the operating manual	9
	1.2	Fur	ther applicable documents	9
	1.3	Inte	nded use	9
	1.3	3.1	Freeze-drying of solvent-containing products (non-aqueous media)	11
	1.3	3.2	Freeze-drying of acid-containing products	12
	1.3	3.3	Freeze-drying of azide-containing products	12
	1.4	Wa	rranty and liability	12
	1.5	Cop	pyright	13
	1.6	Exp	lanation of symbols	13
	1.7	Sta	ndards and regulations	13
	1.8	Sco	pe of supply	13
2	L	ayou	t and mode of operation	14
	2.1		out of the freeze-dryer	
	2.1	•	Functional and operating elements	
	2.1	.2	Name plate	17
	2.2	Мо	de of operation	18
	2.2	2.1	General information on freeze-drying	18
	2.2	2.2	Freeze-drying process	20
	2	2.2.2.1	Preparation	20
	2	2.2.2.2	Preezing	21
	2	2.2.2.3	B Main drying	21
	2	2.2.2.4	Final drying	22
	2	2.2.2.5	End of drying and aeration	22
	2	2.2.2.6	Defrosting	22
3	S	afety		23
	3.1	Mai	king of the unit	23
	3.2	Exp	lanation of the symbols and notes	24
	3.3	Res	sponsibility of the operator	25
	3.3	3.1	Freeze-drying of solvent-containing products	26
	3.4	Red	quirements concerning the personnel	27
	3.5	Info	rmal safety notes	28
	3.6		ety notes concerning the transport, set-up and connection and initial start-up of the start-up	
	3.6		General hazards	
	3.6	5.2	Hazards caused by improper transport	29
	3.6	5.3	Hazards caused by improper set-up	29
	3.6	5.4	Hazards caused by improper connection	29
	3.6	5.5	Hazards during the initial start-up	29



#### **Table of contents**

	3.7	Safety notes concerning the operation	30
	3.7.	.1 Hazards caused by electricity	30
	3.7.	.2 Hazards caused by natural, flammable refrigerants	30
	3.7.	.3 Hazards caused by nitrogen	31
	3.7.	.4 Hazards caused by harmful products	31
	3.7.	, ,	
	3.7.	, ,	
	3.7.	'	
	3.7.	,	
	3.7.	.9 Oil-sealed vacuum pump: hazards caused by contaminated vacuum pump exhaugases	
	3.7.		p oil
	3.7.		
	3.7.	.12 Hazards caused by noise	34
	3.7.	.13 Hazards caused by the loading door	35
	3.7.	.14 Hazards caused by hot surfaces	35
	3.7.	.15 Hazards caused by cold surfaces	35
	3.7.	.16 Hazards caused by overpressure in the chamber	36
	3.8	Safety devices	36
	3.9	Procedures in the event of hazards and accidents	37
	3.10	Maintenance and cleaning of the freeze-dryer	38
	3.11	Additions or conversions of the freeze-dryer	38
	3.12	Measures to be taken to ensure safe operation of the freeze-dryer	38
	3.13	Remaining hazards	40
4	Sf	torage and transport	41
	4.1	Dimensions and weight	
	4.2	Storage conditions	
	4.3	Unpacking the freeze-dryer	
	4.4	Transport	
	4.4.	·	
5		et-up and connection	
J	5.1	Installation site	
	5.2	Supply and disposal connections	
	5.2	11.7	
	_	.2.1.1 Connection	
	_	.2.1.2 Customer-provided fuses	
	5.2.	·	
	5.2.		
		.2.3.1 Oil-sealed vacuum pump with exhaust filter (oil mist separator)	
		.2.3.2 Dry-running vacuum pump with silencer	
	5.2.		
	5.2.		
	5.2.		



#### **Table of contents**

6	O	peration		53
	6.1	Initial st	art-up	53
	6.2	Installat	tion of accessories	53
	6.3	Prepara	ation	53
	6.4	Switchir	ng the freeze-dryer on	53
	6.5	Loading	g door	54
	6.6	LSCplu	s control system	56
	6.6.	1 Use	r interface	56
	6.	6.1.1	Main window "Manual"	57
	6.	6.1.2	Main window "Program"	70
	6.	6.1.3	Main window "Options"	71
	6.	6.1.4	Main window "?"	86
	6.6.	2 Man	ual freeze-drying	86
	6.	6.2.1	Entering set values in the manual mode	87
	6.6.	3 Free	ze-drying with the PGMplus programmer module	89
	6.	6.3.1	Creating a program	93
	6.	6.3.2	Editing a program	. 101
	6.	6.3.3	Copying a program	
	6.	6.3.4	Loading a program	.102
	6.	6.3.5	Deleting a program	.103
	6.7	Optiona	al extensions and special equipment	.104
	6.8	Switchir	ng the freeze-dryer OFF	. 107
7	Ma	alfunctio	ons and error correction	108
	7.1	Genera	I malfunctions	108
	7.1.	1 Pow	er failure	.109
	7.1.	2 Insu	fficient vacuum	.110
	7.	1.2.1	Small flange connections	.110
	7.	1.2.2	Aeration valve	. 111
	7.	1.2.3	Pressure control valve	.111
	7.	1.2.4	Rubber valves	.111
		1.2.5	Vacuum sensor	
	7.1.	3 Insu	fficient ice condenser temperature	.112
	7.2	Process	s and error messages	.112
	7.3	Service	contact	.113



#### **Table of contents**

8	Mai	ntenance and service	114
8.1	N	Maintenance	114
8	.1.1	General	114
8	.1.2	Chamber	115
	8.1.	2.1 Lamination of the loading door with a special film	116
	8.1.	2.2 Door latch	117
8	.1.3	Aeration valve	
8	.1.4	Heat exchanger (only air-cooled freeze-dryers)	
	.1.5	Electrical system	
	.1.6	Vacuum system with an oil-sealed vacuum pump	
_	.1.7	Vacuum system with a dry-running vacuum pump	
_	1.8	Refrigeration system	
_	1.1.9	Vacuum sensor	
		) Accessories	
8.2		Disinfection of the drying chamber and accessories	
8.3		Maintenance schedule (oil-sealed vacuum pump)	
8.4		Maintenance schedule (dry-running vacuum pump)	
8.5		Service	
8.6		Return of defective parts	
9	-	posal	
9.1		Disposal of the freeze-dryer	134
9.2		Disposal of the packaging	134
10	Tec	hnical data	135
10.	1 /	Ambient conditions	136
10.	2 1	Fechnical documentation	136
11	App	oendix	137
11.	1 N	Mathematical relations	137
11.	2 E	EC declaration of conformity in accordance with the EC Machinery Directive	139
11.	3 l	JKCA declaration of conformity	141
11.	4 E	EC declaration of conformity in accordance with the Pressure Equipment Directive	143
11.		Fable of the sublimation pressure curve	
12		ssary	
13		ex	



#### 1 General information

# 1.1 Importance of the operating manual

A fundamental requirement for the safe and trouble-free operation of the unit is to be familiar with the fundamental safety instructions and all possible hazards.

The operating manual includes important information concerning the safe operation of the freeze-dryer.

This operating manual, and in particular the notes on safety and hazards, must be observed by all persons operating the unit.

In addition, the local rules and regulations for the prevention of accidents must be complied with.

# 1.2 Further applicable documents

The following documents apply in addition to these operating instructions if the freeze-dryer is equipped with the corresponding features:

 Operating instructions of the CHRIST SCADA software LPCplus (instructions for the operation of the freeze-dryer by way of a SCADA system)

#### 1.3 Intended use

#### Freeze-dryer

Do not use the freeze-dryer unless the following requirements are fulfilled:

- The freeze-dryer has been properly installed.
- The freeze-dryer is in a perfect technical state.
- The freeze-dryer is not located in an area with an explosion hazard.
- No unauthorised design modifications, additions or conversions without the written approval by Martin Christ Gefriertrocknungsanlagen GmbH have been performed.
- The vacuum pump used is approved by Martin Christ Gefriertrocknungsanlagen GmbH. The vacuum pumps approved for this system are listed in (see chapter 5.2.3 - "Vacuum pumps").
- The accessories used have been approved by Martin Christ Gefriertrocknungsanlagen GmbH. This does not apply to commercially available freeze-drying vessels made of glass or plastic.

The freeze-dryer has been exclusively designed for the freeze-drying of solid or liquid products in ampoules, vials or dishes. It is, therefore, solely intended for this application.





All of the process steps that are necessary for freeze-drying as well as any necessary auxiliary processes (venting, defrosting, draining of media, leak tests) can be performed in the system:

- Freezing of the products with time and temperature setpoints that can be preset as desired
- Main drying of the products with time, temperature and pressure setpoints (→ Sublimation) that can be preset as desired
- Secondary drying of the products with time and temperature setpoints that can be preset as desired, and with a high final vacuum for eliminating any water that is bound by capillary or molecular effects (→ desorption).

The freeze-dryer is suitable for freeze-drying solid substances and aqueous solutions (e.g. bacteria and virus cultures, blood plasma, serum fractions, antibodies, sera, vaccines and pharmaceutical products such as chloramphenicol, streptomycin, vitamins, ferments and plant extracts for biochemical tests).

#### The intended use also includes:

- Observation of all of the notes and instructions that are included in the operating manual (see chapter 1.2 - "Further applicable documents")
- Compliance with the inspection and maintenance instructions (see chapter 8 "Maintenance and service").

#### **Exclusion of liability**

Any use of the freeze-dryer other than the one described here or any use going beyond this description is regarded as improper use. Martin Christ Gefriertrocknungsanlagen GmbH cannot be held liable for any damage resulting from such improper use.

#### Requirements concerning the products used in the freeze-dryer

- The product must not damage the material of the components of the freeze-dryer or affect its mechanical strength.
- A reaction of the product following the supply of high amounts of energy during the freeze-drying process must be excluded.
- The product must not be explosive or highly flammable since certain components of the freeze-dryer are a potential source of ignition.



The additional information concerning special products in the following chapters must be absolutely observed (see chapter 1.3.1 - "Freeze-drying of solvent-containing products (non-aqueous media)", chapter 1.3.2 - "Freeze-drying of acid-containing products", chapter 1.3.3 - "Freeze-drying of azide-containing products")!



#### 1.3.1 Freeze-drying of solvent-containing products (non-aqueous media)

With regards of corrosion resistance, the use of some organic solvents in aqueous solutions with low concentrations is acceptable.

A freeze-dryer is designed to be chemically resistant to most compounds that are commonly used in freeze-drying processes. However, by necessity, the freeze-dryer is comprised of several different materials, some of which may be attacked and degraded by certain chemicals.

The methods of fabrication and/or conditions of exposure of an acrylic door, as well as the way the chemicals are applied, can influence the results. Some of these factors are listed below:

- Fabrication: Stress generated while sawing, sanding, machining, drilling, polishing, and/or forming.
- Exposure: Length of exposure, stresses induced during the life of the product due to various loads, changes in temperature etc.
- Application of chemicals: by contact, rubbing, wiping, spraying etc.

The following table can be used as a general guide for the expected degradation during normal freeze-drying processes of organic solvents with a total max. concentration of 10 vol-% in aqueous solutions.

Solvent	Acrylic glass	Stainless steel	Silicon rubber	EPDM
Acetic acid 20%	+	+	+	0
Formic acid up to 10%	+	0	0	-
Trifluoracetic acid (TFA)	-	+	0	+
Calcium chloride	+	+	+	+
Sodium phosphate	+	+	-	+
Acetone	-	+	+	+
Acetonitrile	-	+	-	0
Carbon tetrachloride	-	+	-	-
Cyclohexane	+	+	-	-
Dioxane	-	+	-	0
Methyl-t-butyl ether	+	+	0	-
Pyridine	-	+	-	0
Methanol	-	+	+	+
Ethanol	0	+	0	+
tert-Butanol	-	+	-	0
DMSO	-	+	-	+

Legend:

- + No degradation to be expected
- o Moderate degradation; limited use
- Severe degradation; infrequent use recommended; immediate thorough cleaning required



#### 1 General information

The chemical attack on devices and accessory components can be significantly reduced by immediate cleaning after the end of operation. All parts of the freeze-dryer that have come in contact with the product must be checked regularly for damages and replaced if necessary.



Solvents that are not listed in the table above, or the listed solvents in a concentration higher than 10% by volume, must not be used!

#### 1.3.2 Freeze-drying of acid-containing products

Freeze-drying of products containing acids (with the exception of the substances already listed under chapter 1.3.1 - "Freeze-drying of solvent-containing products (non-aqueous media)" in the concentrations stated there) is only permissible if special protective measures and equipment-related precautions are taken. Otherwise, there is a risk of damage to property and personal injury. Consultation of Martin Christ Gefriertrocknungsanlagen GmbH is absolutely mandatory in order to define the measures that need to be taken!

#### 1.3.3 Freeze-drying of azide-containing products

Freeze-drying of products containing azides is only permissible following a case-by-case examination and the written approval by Martin Christ Gefriertrocknungsanlagen GmbH, since azides may form explosive dust-air-mixtures and also explosive metal azides when combined with non-ferrous metals (e.g. copper, brass, bronze)!

# 1.4 Warranty and liability

The warranty and liability are subject to our "General Terms and Conditions" that were distributed to the operator upon the conclusion of the contract.

Warranty and liability claims are excluded if they are due to one or several of the following reasons:

- improper use
- non-compliance with the safety instructions and hazard warnings in the operating manual
- improper installation, start-up, operation, and maintenance of the freeze-dryer.



## 1.5 Copyright

The copyright concerning the operating manual remains with Martin Christ Gefriertrocknungsanlagen GmbH.

The operating manual is solely intended for the operator and their personnel. It includes instructions and information that may not be

- · duplicated,
- · distributed, or
- communicated in any other way neither in full nor in parts.

Non-compliance may be prosecuted under criminal law.

## 1.6 Explanation of symbols

In this operating manual, specialist terms that are explained in the glossary (see chapter 12 - "Glossary") are marked by an arrow and printed in italics (e.g.  $\rightarrow$  sublimation).

# 1.7 Standards and regulations

EC declaration of conformity in accordance with the EC Machinery Directive and EC declaration in accordance with the Pressure Equipment Directive (see chapter 11.2 - "EC declaration of conformity in accordance with the EC Machinery Directive" and chapter 11.4 - "EC declaration of conformity in accordance with the Pressure Equipment Directive").

# 1.8 Scope of supply

According to your order, our order confirmation, and our delivery note.



# 2 Layout and mode of operation

# 2.1 Layout of the freeze-dryer

#### 2.1.1 Functional and operating elements

- Control system
- 2 Opening for the standard option sealing device
- 3 Drying chamber with loading door and locking handle



Fig. 1: Overview of the freeze-dryer

- 4 Connections for the product sensors and a LyoRX sensor
- 5 Shelf
- 6 Door latch
- 7 Ice condenser
- 8 Defrosting water collecting tray

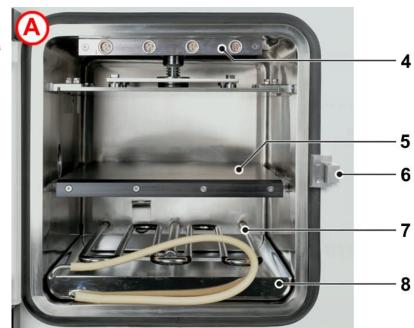


Fig. 2: Detailed view A - drying chamber



#### 9 Control switch



Fig. 3: Right side of the freeze-dryer

- 10 Aeration valve
- 11 Access flange DN40 (e.g. for standard option "WTMplus", behind the side panel)



Fig. 4: Left side of the freeze-dryer



#### 2 Layout and mode of operation

- 12 Name plate
- 13 Heat exchanger for the heat transfer medium (behind the panel)
- 14 Vacuum connection



Fig. 5: Rear view of the freeze-dryer

- 15 Connection for a Pirani vacuum sensor
- 16 Ethernet connection
- 17 Connection for a capacitive vacuum sensor
- 18 USB connection (only in function if the standard option "USB process recording" is installed)

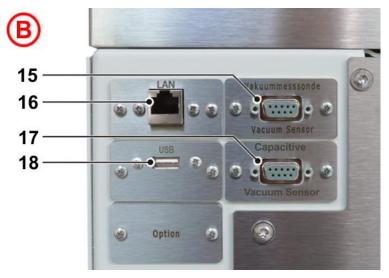


Fig. 6: Detailed view B - Connections on the rear side of the freeze-dryer



- 19 Vacuum sensor connection
- 20 Internal fuse
- 21 Power supply of the pressure control valve
- 22 Power supply of the vacuum pump
- 23 Automatic circuit breaker 1F1
- 24 Equipotential bonding screw (hidden by the mains cable)

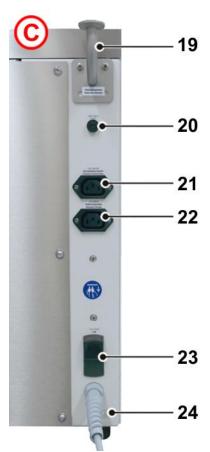


Fig. 7: Detailed view C – Connection bar on the rear side of the freeze-dryer (see chapter 2.1.2 - "Name plate")

#### 2.1.2 Name plate

- 1 Serial number
- 2 Type
- 3 Refrigerant data of the 1<sup>st</sup> stage
- 4 Nominal voltage
- 5 Year of manufacture (month/year)
- 6 Part number
- 7 Refrigerant data of the 2<sup>nd</sup> stage
- 8 Rated current / apparent power



Fig. 8: Example of a name plate (here: Epsilon 2-4 LSCplus)



### 2.2 Mode of operation

#### 2.2.1 General information on freeze-drying

#### What is freeze-drying?

Freeze-drying or lyophilisation is a procedure for the gentle drying of high-quality products. The product is dried by  $\rightarrow$  *sublimation* without passing through the liquid phase.

#### What are typical applications for freeze-drying?

An important area of application is the drying of biotechnological and pharmaceutical products, e.g. tissues and tissue extracts, bacteria, vaccines, and sera. Products that would not keep well when they are dissolved in water can be preserved by freeze-drying. During this process, the biological properties of these sensitive substances are preserved. The compounds remain unchanged from a qualitative and quantitative point of view. After the addition of water, the products will have the same characteristics as the original products.

#### How does freeze-drying work?

Freeze-drying is a very gentle procedure for the extraction of water from a product in the frozen state. The drying process takes place through  $\rightarrow$  *sublimation*, i.e. the direct transition of a product from the solid phase to the gas phase. This happens under vacuum.

The following section describes the process of sublimation based on the example of water, since most products that are processed by freeze-drying are aqueous solutions. Their behaviour is based on identical fundamental principles.

The vapour pressure curve for ice and water (sublimation pressure curve) describes the phase transition as a function of the pressure and temperature. The higher the temperature is, the higher the vapour pressure.

- If the vapour pressure is higher than 6.11 mbar (A), water passes through all three phases: solid, liquid, and gas (see the illustration).
- At 6.11 mbar and 0.0098°C, the melting pressure curve, vapor pressure curve, and sublimation pressure curve meet in one point, the so-called triple point. In this point, all three phases coexist (simultaneously).
- If the vapour pressure is below 6.11 mbar (B) and energy is added, the ice will be directly converted into water vapour once the sublimation curve is reached. This transition is called "sublimation". If thermal energy is added to pure ice with a temperature of less than -30°C at a pressure of 0.37 mbar, it will be converted into water vapour once it reaches -30°C (see figure).

The vacuum prevents the melting of ice when energy is added. If thermal energy is added to a frozen product under vacuum, thawing of the product will be prevented and the water that is contained within the product will be released in the form of water vapour.





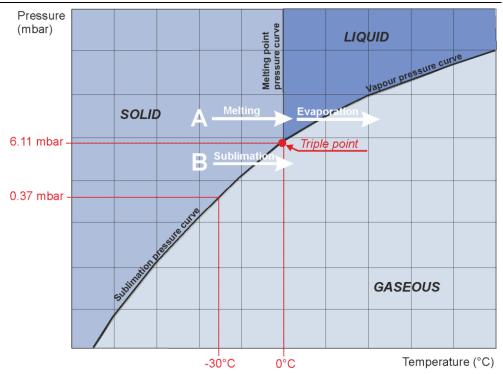


Fig. 9: Vapour pressure curve for ice and water

From a physical point of view, the freeze-drying process covers three phases (see figure below):

- (1) Freezing: The product to be dried is frozen under atmospheric pressure. This can be done either directly in the freeze-dryer or in a separate deepfreeze. The freezing temperature should be approximately 10°C below the solidification point of the product.
- (2) Evacuation: When the product is sufficiently frozen, the vacuum pump is activated. The pressure inside the drying chamber will be lowered to the value that corresponds to the freezing temperature in accordance with the vapour pressure curve for ice and water.
- (3) Sublimation: Thermal energy is added to the product, thus starting the sublimation process. Due to the added energy, the water in the product is converted into water vapour. Since the ice condenser is much colder than the product that is to be dried, the vapour pressure in the ice condenser is considerably lower than above the product. As a result, the water vapour that is released by the product streams to the ice condenser, where it condenses on the condenser coils.

Once the free water has been extracted from the product during the main drying phase, the last traces of bound water will also be removed at a final pressure that is as low as possible and at higher temperatures. This takes place by way of  $\rightarrow$  desorption. This drying phase is also called final drying.



#### 2 Layout and mode of operation

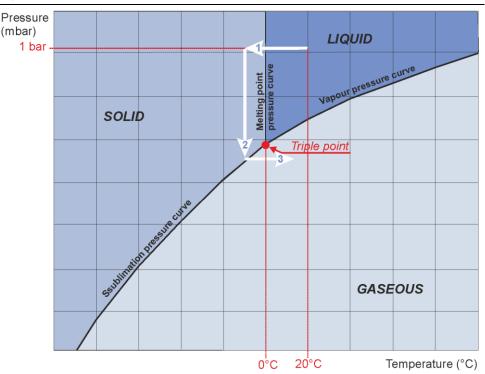


Fig. 10: Freeze-drying phases



Please find further information about basic principles, optimum procedures and applications in the brochure "Smart freeze-drying", which can be downloaded at <a href="https://www.martinchrist.de">www.martinchrist.de</a>  $\rightarrow$  [Applications]  $\rightarrow$  [Lyophilisation].

#### 2.2.2 Freeze-drying process

The main components of a freeze-dryer are:

- vacuum drying chamber or drying manifold,
- vacuum pump for generating a vacuum inside the drying chamber,
- ice condenser for binding the water vapour that is released by the product.

#### 2.2.2.1 Preparation

The ice condenser chamber must be clean and dry. Any water residues from a preceding drying run must be removed.

The media drain valve and the aeration valve must be closed.

In the case of units that are equipped with a pressure control valve (standard on LSCplus and LSCbasic units), the vacuum pump should be warmed up ("warm-up") for at least 15 minutes prior to the start of the main drying phase. Do not subject the vacuum pump to condensable gases until the operating temperature is reached. In this way, the service life of the vacuum pump can be extended.

At the same time, the ice condenser is pre-cooled ("cool-down"). The ice condenser temperature does not have any influence on the product temperature. The sole purpose of the ice condenser is to bind the released water vapour.



#### 2.2.2.2 Freezing

First, the product that is to be dried is frozen. This can be carried out either directly in the freeze-dryer or in a separate deep-freeze. Especially in the case of small filling quantities, we recommend pre-cooling the shelves as well in order to prevent the product from thawing during the evacuation.

Two very different structures of the frozen material can be distinguished:

- · crystalline structures with clearly distinguishable crystals
- amorphous structures with no crystal junctions at all (e.g. glass)

The majority of the freeze-drying products have a crystalline form.

When freezing these kinds of products, one must take into consideration that too deep and too quick freezing leads to smaller ice crystals, which has a negative effect on the duration of the drying process.

For every product to be dried, the solidification point must be determined as a first step. This is the point at which the water that is contained in the product has completely crystallised. In order to ensure an optimum freezedrying process, the product temperature should be approximately 10°C below the solidification point.

#### 2.2.2.3 Main drying

When the product is frozen, the main drying phase commences. The vacuum pump is switched on. The pressure inside the drying chamber will be lowered to the value that corresponds to the freezing temperature in accordance with the vapour pressure curve for ice and water (sublimation pressure curve). At the same time, thermal energy will be added to the product. In the case of products in round-bottom flasks, wide-neck bottles, etc., this is realised through the environment that is considerably warmer (direct contact heat), in the case of unheated shelves by way of thermal radiation from the environment, and in the case of temperature-controlled shelves directly via the shelves. As a result, the sublimation process starts. At the beginning of the drying process, the maximum drying rate will be reached. The more the sublimation area recedes into the product, the further the produced water vapour must pass through the layers that have already been dried.

Under certain conditions, it is possible that the vacuum inside the ice condenser chamber increases during the main drying phase (e.g. from 0.63 mbar to 0.47 mbar) although the valve towards the vacuum pump is closed. From a physical point of view, this is due to the pumping effect of the ice condenser ("cryo-pumping effect").

The required drying time depends strongly on the drying vacuum. At 1.0 mbar, one gram of ice takes up a volume of 1 m³ of vapour, at 0.1 mbar a volume of 10 m³ of vapour, and at 0.001 mbar a volume of 100 m³. The closer the vacuum is to the solidification point, the smaller is the resulting vapour volume. The drying rate increases and the drying time decreases.

#### 2 Layout and mode of operation



#### 2.2.2.4 Final drying

Final drying is an option whenever one requires a product with minimal residual moisture. In the physical sense, this process is a desorption process, i.e. the removal of adsorptively bound water. Final drying is performed under the lowest possible final pressure that depends on the ice condenser temperature in accordance with the vapour pressure curve for ice and water as well as on the final vacuum of the vacuum pump that is used. The process is supported by a higher shelf temperature.

#### 2.2.2.5 End of drying and aeration

The end of the drying process is reached when both the product and shelf temperature are clearly in the positive range (+15 to +20°C) and if their difference is not greater than 5 K.

Another indication of the end of the drying process is the behaviour of the vacuum and of the ice condenser temperature. The ice condenser is no longer subject to load and reaches the final temperature of approximately -55°C or -85°C. The pressure in the drying chamber decreases in accordance with the ice condenser temperature.

The vacuum pump will be switched off and the drying chamber will be aerated via a rubber valve or via the aeration valve. The aeration valve can also be used to flood the unit with nitrogen or another inert gas instead of ambient air.

Then, the product can be removed from the unit.

#### 2.2.2.6 Defrosting

#### **Defrosting with hot gas**

As standard, the freeze-dryer is equipped with a hot-gas defrosting system. In order to defrost the ice condenser, heated refrigerant is fed through the heating coil. In addition, the bottom of the ice condenser chamber is heated by way of a heating collar.


In order to avoid damage, the condensate must be drained off through the media drain valve directly after the completion of the defrosting process. Then, any residual water must be removed from the ice condenser chamber by way of a cloth.




# 3 Safety

# 3.1 Marking of the unit

The following symbols are used for Christ freeze-dryers:

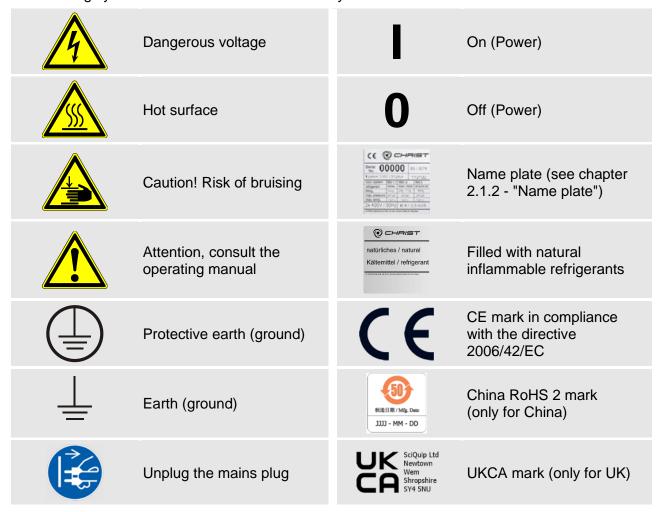

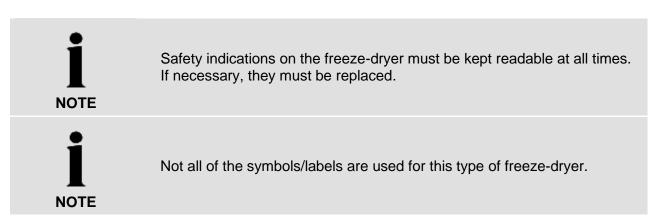



# 3.2 Explanation of the symbols and notes

This operating manual uses the following names and symbols to indicate hazards:



This symbol stands for a **direct** hazard to the life and health of persons.

Non-observance of these symbols <u>causes</u> serious health problems up to life-endangering injuries.



This symbol stands for a <u>direct</u> hazard to the life and health of persons due to electrical voltage.

Non-observance of these symbols <u>causes</u> serious health problems up to life-endangering injuries.



This symbol stands for a **potential** hazard to the life and health of persons.

Non-observance of these symbols <u>can</u> cause serious health problems up to life-endangering injuries.



This symbol indicates a potentially hazardous situation

Non-observance of these notes can cause minor injuries or damage to property.



This symbol indicates important information.



## 3.3 Responsibility of the operator

The operator is the person who uses the freeze-dryer for commercial or economic purposes or lets a third party use it and who bears the legal product responsibility for the protection of the users, personnel or third parties during operation.

#### **Operating personnel**

The operator is obliged to ensure that

- the persons working on/with the freeze dryer
  - are 18 years old or older,
  - have been specifically ordered to operate the system by the operator,
  - have been trained in terms of the operation of this system,
  - have been duly informed about the specific hazards associated with the system, supply media and starting/final products as well as about the correct conduct and necessary measures to take in the event of accidents or malfunctions,
  - are familiar with the fundamental health, safety and accident prevention regulations,
  - have read and understood this operating manual (in particular the safety sections and warning notes) as well as any additional applicable documents (see chapter 1.2 - "Further applicable documents") and confirmed this with their signature.
- the areas of responsibility of the personnel concerning the operation, maintenance and care of the unit are clearly defined.
- standard operating procedures (SOPs) concerning the various products that are freeze-dried in the freeze-dryer are provided (see the section below "Work area").
- the safety-conscious work of the personnel in compliance with the operating manual and the relevant EC health and safety directives and the national laws concerning health and safety and the prevention of accidents are checked at regular intervals (e.g. every month).

#### Work area

The operator must

- perform a risk assessment concerning potential accidents in connection with the freeze-dryer and take design-related countermeasures, if necessary.
- check the sound pressure level at the workplace of the operating
  personnel after the setup of the freeze-dryer. The sound pressure level
  depends on the local conditions (e.g. sound reflected from the ceiling
  and surrounding walls, external sources of noise). If necessary, the
  operating personnel must wear suitable personal protective equipment
  or other suitable protective measures must be taken in line with the
  applicable legal provisions in order to avoid noise-induced hearing loss.
- perform a risk assessment in view of the specific hazards associated with specific products that are freeze-dried in the freeze-dryer (e.g. ignition/explosion hazard, discharge of harmful product residues at the outlets of the chamber) and take the corresponding measures, if necessary.



- perform a compatibility test of all the substances that are used in the freeze-dryer (products to be dried as well as cleaning agents, etc.) and that come into contact with the chamber walls, shelves, pipes/hoses and seals. Substances that damage the material or weaken the mechanical strength must not be used.
- ensure that the freeze dryer is operated with one of the vacuum pumps approved by Martin Christ Gefriertrocknungsanlagen GmbH (see chapter 5.2.3 - "Vacuum pumps").
- have the system maintained at regular intervals (see chapter 8 -"Maintenance and service").
- check the safety devices regularly to ensure their correct operation (see chapter 3.8 "Safety devices").
- replace without delay any parts or components that are not in perfect working order.

#### 3.3.1 Freeze-drying of solvent-containing products

With regards of corrosion resistance, the use of some organic in aqueous solutions with low concentrations is acceptable.

Under certain circumstances, the freeze-drying of products containing solvents may lead to the formation of explosive mixtures. This is why the operator must draw up special operating instructions/SOPs including precise instructions

- concerning the deactivation of specific components (see chapter 1.3.1 "Freeze-drying of solvent-containing products (non-aqueous media)"),
- concerning the inspection of the freeze-dryer in view of damage caused by the solvent that is used (see chapter 1.3.1 - "Freeze-drying of solvent-containing products (non-aqueous media)").

The operator ensures sufficient air exchange in the room where the freezedryer is used if nitrogen is used as the aeration/inertisation medium.



## 3.4 Requirements concerning the personnel



#### Risk of injury if the personnel are not sufficiently qualified

If unqualified personnel perform work on the freeze-dryer or are present in the danger zone of the freeze-dryer, hazards result that can cause serious injuries and considerable damage to property.

- Ensure that all the tasks are performed by personnel with the corresponding qualifications.
- Ensure that unqualified personnel stay clear of the danger zones.



# Risk of fatal injury to unauthorised persons due to hazards in the danger zone or work area

Unauthorised persons who do not fulfil the requirements described herein are not aware of the hazards in the work area. This is why there is a risk of serious or even fatal injuries for unauthorised persons.

- Ensure that unauthorised persons stay clear of the danger zone and work area.
- If in doubt, address these persons and instruct them to leave the danger zone and work area.
- Interrupt any running work if unauthorised persons are present in the danger zone or work area.

This manual uses the following personnel qualifications for various areas of activity:

#### **Operating personnel (users)**

The operating personnel operates and monitors the freeze-dryer during normal operation and within the framework of its intended use. In the event of malfunctions or other problems, the operating personnel informs the respective specialised personnel.

It must be ensured that the persons operating the system

- are 18 years old or older,
- have been specifically ordered to operate the system by the operator,
- · have been trained in terms of the operation of this system,
- have been duly informed about the specific hazards associated with the system, supply media and starting/final products as well as about the correct conduct and necessary measures to take in the event of accidents or malfunctions.
- are familiar with the fundamental health, safety and accident prevention regulations,
- have read and understood this operating manual (in particular the safety sections and warning notes) as well as any additional applicable documents (see chapter 1.2 - "Further applicable documents")and confirmed this with their signature.

#### Specialised personnel

Due to their special training, knowledge, experience and familiarity with the relevant regulations, specialised personnel are in the position to perform any tasks assigned to them and to autonomously identify and prevent possible hazards.



#### **Qualified electrician**

Due to their special training, knowledge, experience and familiarity with the relevant standards and regulations, qualified electricians are in the position to perform work on electrical systems and to autonomously identify and prevent possible hazards.

# 3.5 Informal safety notes

This operating manual is part of the product.

- This operating manual must be kept at the location of use of the freezedryer. Ensure that it is accessible at all times.
- The operating manual must be handed over to every subsequent owner or user of the freeze-dryer.
- Any changes, additions or updates received must be added to the operating manual.
- In addition to the operating manual, the general and operational rules and regulations for the prevention of accidents and the protection of the environment must be provided.
- All of the safety and hazards notes on the freeze-dryer must be kept readable at all times. If necessary, they must be replaced.

# 3.6 Safety notes concerning the transport, set-up and connection and initial start-up of the freeze-dryer

The following notes and instructions must be observed in order to protect all persons and property.

#### 3.6.1 General hazards



#### General risk of injury

Among the general hazards during the transport, set-up and connection and start-up of the freeze-dryer are impact hazards, crushing hazards, grazing hazards, cutting hazards, etc.

This may lead to severe injuries.

- Comply with the fundamental health and safety rules and regulations as well as with the rules and regulations for the prevention of accidents!
- Wear personal protective equipment (safety shoes, work gloves, and hardhat)!



#### 3.6.2 Hazards caused by improper transport



#### Risk of injury caused by the uncontrolled movement of loads

Units or components that are not properly fastened or secured may shift, or fall over.

This may lead to severe damage to health or even life-threatening injuries.

- Take the centre of gravity of the load in consideration (off-centre)!
- Prior to transporting or setting-up the freeze-dryer, read the chapter 4 -"Storage and transport" thoroughly!

#### 3.6.3 Hazards caused by improper set-up



#### Risk of injury caused by poor accessibility of the freeze-dryer

In cramped spaces or locations with poor accessibility, sharp edges and corners may protrude into the work area.

This may lead to injuries caused by impact hazards or grazing hazards.

- Ensure that the freeze-dryer is set up freely accessible!
- Comply with the fundamental health and safety rules and regulations as well as with the rules and regulations for the prevention of accidents!

#### 3.6.4 Hazards caused by improper connection



# Risk of injury caused by escaping media or other consequences of improper connections

Improper connections may lead to problems, e.g. a hazardous electrical incident or the escape of media (depending on the configuration of the freeze-dryer e.g. hot water, nitrogen, hydrogen peroxide), at a later time during the operation of the freeze-dryer.

This may lead to severe damage to health or even life-threatening injuries.

- Ensure that the supply and disposal connections are established by competent and specialised persons under consideration of the corresponding connection specifications (see chapter 5.2 - "Supply and disposal connections" and chapter 10 - "Technical data")!
- The connections to the on-site pipes must be force-free and torquefree!

## 3.6.5 Hazards during the initial start-up



# Risk of injury caused by consequences of transport damage, or improper connections (e.g. escaping media).

Leaks after the transport, set-up, and connection of the freeze-dryer may lead to problems, e.g. the escape of media (depending on the configuration of the freeze-dryer, e.g. refrigerant, heat transfer medium, hydraulic oil, nitrogen, hydrogen peroxide, etc.), at a later time during the initial start-up of the freeze-dryer.

This may lead to severe damage to health or even life-threatening injuries.

 Prior to the initial start-up of the freeze-dryer, all of the supply and disposal connections must be checked for leaks by specialised persons.



## 3.7 Safety notes concerning the operation

The following notes and instructions concerning the operation of the freezedryer must be observed in order to protect all persons and property.

#### 3.7.1 Hazards caused by electricity



#### Danger of life caused by electric shock

There is a risk of electric shock when touching current-carrying components.

This may lead to ventricular fibrillation, cardiac arrest, or respiratory paralysis.

- Only qualified electritians are authorised to perform work on the electrical system of the freeze-dryer!
- The electrical equipment of the freeze-dryer must be checked at regular intervals by a qualified electrician!
- Defects such as loose connections or burnt cables must be eliminated immediately.

#### 3.7.2 Hazards caused by natural, flammable refrigerants



#### Risk of suffocation caused by the refrigerant

When work is performed on the refrigeration system of the freeze-dryer, refrigerant may escape in the liquid or gas state and under high pressure. Gaseous refrigerant is heavier than air and high concentration levels of it may collect on the floor or in pits.

There is a risk of suffocation in the case of high concentration levels. Possible symptoms are paralysis and unconsciousness. Affected persons do not notice the fact that they suffocate.

- Only qualified persons are authorised to perform work on the refrigeration system of the freeze-dryer!
- Ensure good aeration/extraction when working on the refrigeration system!



#### Risk of cold burns or frostbite caused by the refrigerant

When work is performed on the refrigeration system of the freeze-dryer, refrigerant may escape in the liquid or gas state and under high pressure. In the case of skin contact with liquid refrigerant, cold burns or frostbite may result.

 Only qualified persons are authorised to perform work on the refrigeration system of the freeze-dryer!



#### Risk of explosion due to refrigerants

The refrigerants used are highly flammable and can form an explosive mixture if their concentration in the ambient air is sufficiently high.

There is an explosion hazard.

- Work on the refrigeration system of the freeze-dryer must only be carried out by qualified specialist personnel who have been trained to handle flammable refrigerants!
- Ensure good ventilation and make sure that no ignition sources (e.g. soldering iron, welding equipment) are present!



#### 3.7.3 Hazards caused by nitrogen



#### Risk of suffocation caused by nitrogen

If the chamber is aerated with nitrogen, the gas may escape through openings in the system (e.g. supply lines that are not properly connected or a loading door that is not closed correctly).

There is a risk of suffocation in the case of high concentration levels. Possible symptoms are paralysis and unconsciousness. Affected persons do not notice the fact that they suffocate.

- Use the freeze-dryer only if it is equipped with pipes that are properly connected!
- Only qualified persons are authorised to perform work on the nitrogen lines of the freeze-dryer!

#### 3.7.4 Hazards caused by harmful products



#### Risk of poisoning/infection caused by the products

When loading and unloading the shelves, the personnel are exposed to the product.

Skin contact or the inhalation of particles may cause severe damage to health depending on the product in question.

- Wear suitable protective clothes, gloves, and respiratory protection or
- · use an isolater sytem on the freeze-dryer!



#### Risk of poisoning/infection caused by the products

When performing maintenance work on parts coming into contact with the product (e.g. all parts inside the chamber, vacuum pump), the personnel may be exposed to product residues.

Skin contact or the inhalation of particles may cause severe damage to health depending on the product in question.

- Take suitable decontamination measures prior to commencing the maintenance!
- Wear suitable protective clothes, gloves, and respiratory protection!

#### 3.7.5 Hazards caused by solvents in the products



#### Explosion hazard caused by solvents in the products

When freeze-drying products containing solvents, gas mixtures may form. These gas mixtures may be ignited on certain components of the freeze-dryer.

There is an explosion hazard.

- Solvents that are not included in the table in chapter 1.3.1 "Freezedrying of solvent-containing products (non-aqueous media)", or the listed solvents in a concentration higher than 10% by volume, must not be used!
- Refer to the safety data sheets of the products that are used!



#### 3.7.6 Hazards caused by acids in the products



#### Risk of injury caused by acids in the products

Products containing acids may damage the material of the components of the freeze-dryer and affect the mechanical strength.

This may lead to severe injuries.

Freeze-drying of products containing acids is only permissible if special protective measures and equipment-related precautions are taken!

Consultation of Martin Christ Gefriertrocknungsanlagen GmbH is absolutely mandatory in order to define the measures that need to be taken!

Refer to the safety data sheets of the products that are used!

#### 3.7.7 Hazards caused by azides in the products



#### **Explosion hazard caused by azides in the products**

Azides form explosive metal azides when they come into contact with non-ferrous metals (e.g. copper, brass, bronze) that may be present in the pipe system or vacuum pump, for example. In addition, explosive dust-air-mixtures may form during the aeration process after the end of the drying phase.

There is an explosion hazard.

 Freeze-drying products containing azides is only permissible with special protective measure and equipment-related precautions (e.g. a special vacuum pump) and following a case-by-case examination and the written approval by Martin Christ Gefriertrocknungsanlagen GmbH!



#### Risk of poisoning caused by azides in the products

When loading and unloading the shelves, the personnel are exposed to the product.

Skin contact or the inhalation of particles may cause severe damage to health. There is a risk of pulmonary oedemas in the case of inhalation.

- Wear suitable protective clothes, gloves, and respiratory protection or
- · use an isolater sytem on the freeze-dryer!



#### Risk of poisoning caused by azides in the products

When performing maintenance work on parts coming into contact with the product (e.g. all parts inside the chamber, vacuum pump), the personnel may be exposed to product residues.

Skin contact or the inhalation of particles may cause severe damage to health. There is a risk of pulmonary oedemas in the case of inhalation.

- Take suitable decontamination measures prior to commencing the maintenance!
- Wear suitable protective clothes, gloves, and respiratory protection!



## 3.7.8 Hazards caused by contaminated condensate (defrosting water)



# Risk of poisoning/infection caused by contaminated condensate (defrosting water)

The condensate may contain harmful substances originating from the product.

Contact with the condensate may cause severe damage to health.

- Ensure the environmentally sound disposal of the condensate in compliance with the local rules and regulations!
- Wear suitable protective clothes, gloves, and respiratory protection when performing any work on the drain system (especially when cleaning the valves and replacing the seals)!

# 3.7.9 Oil-sealed vacuum pump: hazards caused by contaminated vacuum pump exhaust gases



#### Risk of poisoning/infection caused by vacuum pump exhaust gases

The exhaust gases of the vacuum pump may contain harmful substances originating from the product.

Inhalation may cause severe damage to health.

- Use the freeze-dryer only if it is equipped with a pipe that is properly connected to the outlet of the vacuum pump/exhaust filter (oil mist separator) and led to the outside via the roof!
- Depending on the product that is dried in the freeze-dryer, it may be necessary to install a suitable filter system in the exhaust gas pipe!
- Compliance with the local rules and regulations concerning the protection of the environment must be ensured!



# 3.7.10 Oil-sealed vacuum pump: hazards caused by hot and contaminated vacuum pump oil



#### Risk of scalding caused by the vacuum pump oil

When working on the vacuum pump and exhaust gas filter (especially when changing the oil or filter), the maintenance personnel are exposed to the hot vacuum pump oil.

There is a risk of scalding in the event of skin contact.

- · Wear suitable protective clothes and gloves!
- Use a suitable collecting vessel!



#### Risk of poisoning/infection caused by the vacuum pump oil

When working on the vacuum pump and exhaust gas filter (especially when changing the oil or filter), the maintenance personnel are exposed to the vacuum pump oil, which may contain harmful substances originating from the product. In addition, synthetic oils can release toxic fumes when they are ignited or heated above 300°C.

The inhalation of the fums that are released by the oil, or contact with the skin, can cause severe damage to health.

- Wear suitable protective clothes, gloves, and respiratory protection!
- Ensure the environmentally sound disposal of the oil in compliance with the local rules and regulations!
- Do not let the oil come into contact with tobacco products!

#### 3.7.11 Dry-running vacuum pump: hazards caused by contaminated exhaust air



#### Danger of poisoning/infection due to contaminated exhaust air

The exhaust air may contain harmful substances originating from the product.

Contact with particles in the exhaust air (especially by inhalation) may result in severe damage to health.

- Use a silencer with integrated filter elements or depending on the product – guide the exhaust gases from the outlet of the vacuum pump to a suitable treatment system in order to prevent the discharge of harmful substances into the surrounding atmosphere! Compliance with the national rules and regulations for the protection of the environment must be ensured!
- When working on the vacuum system (and especially on the vacuum pump), it may be necessary to wear suitable protective clothes, gloves, and respiratory protection depending on the product!

#### 3.7.12 Hazards caused by noise



#### Risk of noise-induced hearing loss

Depending on the local conditions, a harmful sound pressure level may occur.

High sound pressure levels can cause noise-induced hearing loss.

• Wear suitable personal hearing protection if necessary!



#### 3.7.13 Hazards caused by the loading door



#### Risk of crushing caused by the movement of the loading door

Due to its relative high mass, the movement of the loading door can hardly be slowed down or stopped.

There is a risk of crushing of body parts between the door and the front of the chamber.

- Move the loading door slowly holding the door handle when opening or closing it. Do not hold the door leaf by its edge!
- Lock the door by turning the door handle!

#### 3.7.14 Hazards caused by hot surfaces



#### Risk of burns on hot surfaces

During the operation of the freeze-dryer and half an hour afterwards, the outer surface of the freeze-dryer (especially the pipes and units) may be hot.

There is a risk of burns when touching the surfaces.

- Wear suitable protective clothes and gloves!
- Do not touch the surfaces on purpose!
- Prior to performing any maintenance work on the vacuum pump or the oil mist separator, let the components cool!



#### Risk of burns on hot surfaces

After a drying process, some or all of the surfaces inside the chamber (chamber walls, shelves, intermediate valve, etc.) may still be hot.

There is a risk of burns when touching the surfaces.

- Wear suitable protective clothes and gloves!
- Do not touch the surfaces on purpose!
- Prior to performing any work on the freeze-dryer, let the components cool!

#### 3.7.15 Hazards caused by cold surfaces



#### Risk of freezing to cold surfaces

The shelves and ice condenser coils can already be cold during the loading phase.

There is a risk of freezing to the shelves or ice condenser coils when touching the surfaces.

- · Wear suitable protective clothes and gloves!
- Do not touch the surfaces on purpose!



#### 3.7.16 Hazards caused by overpressure in the chamber



#### Risk of injury caused by bursting of the chamber

The double chamber is designed for vacuum. It is not a pressure vessel! In the event of a malfunction, an impermissible excess pressure may build up in the chamber, which may cause the chamber to burst.

This may lead to life-threatening injuries.

- Do not use the freeze-dryer when it is pressurised (excess pressure)!
- We strongly recommend installing a pressure relief device (e.g. a safety valve or rupture disc) with a sufficient rating.

# 3.8 Safety devices



The safety devices are aimed at protecting the operating personnel. In case of safety devices that are not operating correctly or of safety-relevant operating elements that are not freely accessible, there is a risk of severe damage to health.

- Keep the safety-relevant operating elements freely accessible at all times!
- Do not manipulate, remove, or disable the safety devices in any way!
- Check the correct operation of the safety devices at regular intervals in accordance with the applicable national and international laws, rules, and regulations concerning health and safety and the prevention of accidents!

#### **Control switch**

Position see chapter 2.1.1 - "Functional and operating elements" In order to disconnect the control circuit from the power supply, the control switch must be switched off.

#### Equipotential bonding screw for earth conductor check

For the earth conductor check, there is an equipotential bonding screw on the rear panel of the freeze-dryer. An earth conductor check can be carried out with the aid of a suitable measuring instrument.



## 3.9 Procedures in the event of hazards and accidents

#### Hazardous electrical incident:

 Switch the mains switch off in order to interrupt the power supply completely.

#### Fire:

- A fire in the electrical control system must be extinguished with a CO<sub>2</sub> fire extinguisher!
- Burning oil must be extinguished with a CO<sub>2</sub> fire extinguisher or powder fire extinguisher!

## Unconsciousness/paralysis due to nitrogen or refrigerant:

 While ensuring your own safety (e.g. self-contained breathing apparatus) remove the affected persons to fresh air. Keep them warm and calm. Get medical attention immediately! In case of respiratory arrest, give artificial respiration.

#### **Electric shock:**

While ensuring your own safety, interrupt the circuit as quickly as
possible (mains switch at the right side of the freeze-dryer). Keep the
affected persons warm and calm. Get medical attention immediately!
Check consciousness and breathing continuously. In the case of
unconsciousness of lack of normal breathing, perform cardiopulmonary
resuscitation (CPR).

### **Burns:**

- Cool small-area burns (e.g. finger) immediately with cold water for approximately 2 minutes.
- Do not cool if larger areas of the body surface are burnt since there is a risk of hypothermia.
- Cover the burns loosely and in a sterile manner (e.g. with sterile dressing).
- Keep the affected persons warm and calm.

## **Chemical burns:**

Eyes:

Rinse the eyes thoroughly with plenty of water with the lid gap wide open for at least 15 minutes (eyewash bottle). **Consult an ophthal-mologist immediately** even if there are no immediate symptoms. If possible, continue rinsing the eyes during the transport to the ophthal-mologist.

Respiratory tract:

While using a **suitable breathing apparatus**, remove the affected persons to fresh air. Keep them warm and calm. **Get medical attention immediately!** In case of irregular breathing or respiratory arrest, give artificial respiration.



#### Skin:

Wash with plenty of water. Remove contaminated clothing. Rinse the affected skin areas under flowing water for at least 10 minutes. **Get medical attention immediately!** 

## · Oesophagus:

Do not put anything into the mouth of an unconscious person. Wash the mouth out with water, If the person is conscious: Give the affected person plenty of water to drink (2 glasses maximum). Do not induce vomiting. In case of spontaneous vomiting, keep the head of the affected person lying on his/her stomach low in order to prevent any liquid from entering the respiratory tract. **Get medical attention immediately!** 

IF IN DOUBT; CALL AN EMERGENCY PHYSICIAN!

## 3.10 Maintenance and cleaning of the freeze-dryer

The substances and materials that are used must be properly handled and disposed of (Please refer to the safety data sheets!). This applies particularly to

- · the handling of solvents, lyes, and acids,
- the changing and topping-up of operating supplies.

Compliance with the national rules and regulations must be ensured.

## 3.11 Additions or conversions of the freeze-dryer

Additions or conversions of the freeze-dryer require the written approval by Martin Christ Gefriertrocknungsanlagen GmbH.

## 3.12 Measures to be taken to ensure safe operation of the freeze-dryer

In order to ensure the safe operation of the freeze-dryer, please comply with the following points prior to every freeze-drying process:

#### Set-up, connection and operation

- Ensure that the freeze-dryer was set up and connected properly (see chapter 5 "Set-up and connection").
- Check the freeze-dryer and the accessories before every start-up for any visible signs of damage.
- Do not hit or move the freeze-dryer during its operation.
- Do not lean against or rest on the freeze-dryer during its operation.
- Stop the freeze-dryer immediately in the event of a malfunction.
   Eliminate the malfunction (see chapter 7 "Malfunctions and error correction") or contact the after-sales service of Firma Martin Christ Gefriertrocknungsanlagen GmbH (see chapter 7.3 "Service contact").
- Ensure that all repairs are performed only by authorised and specialised personnel.



## Fire prevention

 Fuses protect certain electrical circuits within the freeze-dryer against over-current conditions. Always use fuses of the same type and rating.

## Safety area

- Maintain a safety distance of at least 30 cm (12 inches) around the freeze-dryer.
- Do not store any dangerous goods in the safety area of the freezedryer.
- Do not place any dangerous material, e.g. glass vessels containing liquid substances, within the safety area of 30 cm around the freezedryer. Spilled liquids may get into the freeze-dryer and damage the electrical or mechanical components.
- Do not stay in the safety area longer than what is absolutely necessary for the operation of the freeze-dryer.

#### **Accessories**

- Do not use the freeze-dryer with accessories that shows signs of damage.
- Only use accessories that have been approved by the manufacturer (except for commercial vessels made of glass or synthetic materials).
   We explicitly warn against the use of equipment of poor quality!
   Breaking glass or bursting vessels can cause dangerous situations.

#### Handling hazardous materials

- The generally applicable regulations for handling flammable substances in laboratories / workplaces must be observed.
- During sample preparation, loading and unloading of samples and defrosting, appropriate safety precautions must be observed.
- Depending on the used solvent, hot gas defrosting should be avoided.
- Caution when handling hazardous materials such as strong acids or bases, radioactive substances and volatile organics: If such substances are spilled, they must be cleaned up immediately.
- If a sample with hazardous materials such as strong acids or bases, radioactive substances or volatile organics is spilled inside a chamber, they must be cleaned up immediately.
- Caution when handling solvents: Keep sources of ignition away from solvents.
- When using flammable or hazardous solvents, the vacuum pump must be vented to or operate inside a fume hood.



## 3.13 Remaining hazards

All Christ freeze-dryers were built state-of-the-art and according to the accepted safety rules. Danger to life and limb of the operator, or of third parties, or impairments of the units or other material assets, however, cannot be completely excluded when the units are being used.

Use the freeze-dryer

- only for the purpose that it was originally intended for (see chapter 1.3 -"Intended use") and
- only if it is in a perfect running state.
- · Immediately eliminate any problems that can affect safety.



## 4 Storage and transport

## 4.1 Dimensions and weight

	EPSILON 1-4 LSCplus	EPSILON 2-4 LSCplus
Height:	520 mm	520 mm
Width:	780 mm	780 mm
Depth:	598 mm incl. vacuum connection	598 mm incl. vacuum connection
Weight:	ca. 110 kg (without vacuum pump)	ca. 140 kg (without vacuum pump)

## 4.2 Storage conditions

In order to ensure the protection against mechanical and climatic influences, the guidelines of the German Federal Association for Wooden Packages, Pallets, and Export Packaging (Bundesverband Holzpackmittel, Paletten, Exportverpackung e.V.), the so-called HPE packaging guidelines, must be applied when packing and storing the freeze-dryer.

The storage must be:

- dust-free
- dry
- free from excessive temperature fluctuations
- · free from a mechanical load.



## 4.3 Unpacking the freeze-dryer



## General risk of injury

Among the general hazards when unpacking or during the transport of the freeze-dryer are impact hazards, crushing hazards, grazing hazards, cutting hazards, etc.

This may lead to severe injuries.

- Comply with the fundamental health and safety rules and regulations as well as with the rules and regulations for the prevention of accidents!
- Wear personal protective equipment (safety shoes, work gloves, and hardhat)!



## Risk of injury caused by the uncontrolled movement of loads

Freeze-dryer components that are not properly fastened or secured may shift, or fall over.

• Take the centre of gravity of the load in consideration (off-centre)!



The freeze-dryer Epsilon 1-4 LSCplus weighs approx. 110 kg! The freeze-dryer Epsilon 2-4 LSCplus weighs approx. 140 kg!

The freeze-dryer is packaged in a wooden crate.

- After opening the packaging, take out the accessories.
- · Remove the packaging material.
- Remove the side walls of the crate.
- Lift the freeze-dryer upwards with a lifting device. Always reach under the freeze-dryer from side.
- Retain the packaging for any possible future transport of the freezedryer.



## 4.4 Transport



#### General risk of injury

Among the general hazards during the transport of the freeze-dryer are impact hazards, crushing hazards, grazing hazards, cutting hazards, etc. This may lead to severe injuries.

- Comply with the fundamental health and safety rules and regulations as well as with the rules and regulations for the prevention of accidents!
- Wear personal protective equipment (safety shoes, work gloves, and hardhat)!



## Risk of injury caused by the uncontrolled movement of loads

Freeze-dryer components that are not properly fastened or secured may shift, or fall over.

• Take the centre of gravity of the load in consideration (off-centre)!



The freeze-dryer Epsilon 1-4 LSCplus weighs approx. 110 kg! The freeze-dryer Epsilon 2-4 LSCplus weighs approx. 140 kg!




Freeze-dryers of the type Epsilon 1-4 LSCplus and Epsilon 2-4 LSCplus that are filled with natural, flammable refrigerants are not approved as air freight!

- Use suitable packaging for the transport, and if at all possible, the original packaging.
- Install all transport safety devices (see chapter 4.4.1 "Transport safety devices").
- Always lift the freeze-dryer with a lifting device.
- When lifting the freeze dryer, always reach under the freeze-dryer from the side. Do not grab the unit at the plastic control panel.
- When setting the unit down, ensure that the feet are upright (see figures below).



Fig. 11: Unit feet (example illustration)







## 4.4.1 Transport safety devices

The following transport safety devices must be removed prior to start-up:

- Install the vacuum sensor (see chapter 5.2.5 "Vacuum sensor").
- Remove the packaging material of the collecting tray in the drying chamber.
- If the freeze-dryer is equipped with a sealing device: Remove the polystyrene blocks between the sealing device and the shelf.



Prior to any transport, the transport safety devices must be reinstalled.



## 5 Set-up and connection



## Risk of injury caused by poor accessibility of the freeze-dryer

In cramped spaces or locations with poor accessibility, sharp edges and corners may protrude into the work area.

This may lead to injuries caused by impact hazards or grazing hazards.

- Ensure that the freeze-dryer is set up freely accessible!
- Comply with the fundamental health and safety rules and regulations as well as with the rules and regulations for the prevention of accidents!



# Risk of injury caused by escaping media or other consequences of improper connections

Improper connections may lead to problems, e.g. a hazardous electrical incident or the escape of media (depending on the configuration of the freeze-dryer e.g. hot water, nitrogen, hydrogen peroxide), at a later time during the operation of the freeze-dryer.

This may lead to severe damage to health or even life-threatening injuries.

- Ensure that the supply and disposal connections are established by competent and specialised persons under consideration of the corresponding connection specifications (see the instructions in this chapter and chapter 10 - "Technical data")!
- The connections to the on-site pipes must be force-free and torquefree!

## 5.1 Installation site

Operate the freeze-dryer only in closed and dry rooms.



Refrigeration problems of the freeze-dryer are often caused by insufficient conditions at the location of use. This is why compliance with the following conditions is absolutely mandatory!

- Ensure sufficient ventilation. Do not place any paper, cloth, or similar material behind or under the unit, since otherwise the air circulation will be impaired.
- Keep a safety distance of at least 30 cm around the freeze-dryer so that the vents in the unit remain fully effective.
- The ambient temperature must be in the range of +5°C to +25°C. A
  potential night-time setback of the air conditioning system must be
  taken into consideration.
- Prevent the room temperature from rising, for example due to closed doors at night.
- Do not subject the freeze-dryer to thermal stress, e.g. by positioning it near heat generators.
- Prevent thermal overload, e.g. caused by other equipment in the direct vicinity of the freeze-dryer.
- Do not set up the vacuum pump directly next to the heat exchanger (condenser).
- Avoid direct sunlight (UV radiation).



## 5.2 Supply and disposal connections

## 5.2.1 Power supply

#### 5.2.1.1 Connection



The operating voltage on the name plate must correspond to the local supply voltage

Christ freeze-dryers are units of safety class I. Epsilon 1-4 LSCplus and Epsilon 2-4 LSCplus units have a three-wire power cord with a CEE 7/4 plug (type F) (see chapter 10 - "Technical data").

## 5.2.1.2 Customer-provided fuses

The freeze-dryer must be protected by way of a customer-provided mains fuse with the correct rating.

#### 5.2.2 Aeration



## Risk of injury caused by bursting of the chamber

The double chamber is designed for vacuum. It is not a pressure vessel! In the event of a malfunction, an impermissible excess pressure may build up in the chamber, which may cause the chamber to burst.

This may lead to life-threatening injuries.

- Do not use the freeze-dryer when it is pressurised (excess pressure)!
- We strongly recommend installing a pressure relief device (e.g. a safety valve or rupture disc) with a sufficient rating.

The freeze-dryer is equipped with one aeration valve (see chapter 2.1.1 - "Functional and operating elements").

After the freeze-drying process, the aeration valve is used for aerating the chambers to atmospheric pressure so that the loading door can be opened in order to remove the product.

Usually, the ambient air is used for the aeration. However, the chamber can also be aerated with an inertisation medium (e.g. nitrogen) via the hose connector of the aeration valve.



## 5.2.3 Vacuum pumps

To ensure their intended use, the freeze-dryers Epsilon 1-4 LSCplus and Epsilon 2-4 LSCplus must be used with one of the following vacuum pumps:

Oil-sealed vacuum pumps:

- Rotary vane pump Vacuubrand RZ6
- Rotary vane pump Vacuubrand RC6
- Rotary vane pump Edwards RV8
- Rotary vane pump Pascal 2010 C1 (only for Epsilon 1-4 LSCplus)

#### Dry vacuum pumps:

- Scroll pump Edwards nXDS 10iC (in the case of Epsilon 1-4 LSCplus only with an external power supply)
- Scroll pump Pfeiffer HiScroll 12 Atex (only for Epsilon 1-4 LSCplus)
- Vacuum pump Vacuubrand VacuuPure 10
   (this pump can only be used to a limited extent as more time is required for the evacuation)

## 5.2.3.1 Oil-sealed vacuum pump with exhaust filter (oil mist separator)



## Risk of poisoning/infection caused by vacuum pump exhaust gases

The exhaust gases of the vacuum pump may contain harmful substances originating from the product.

Inhalation may cause severe damage to health.

- Use the freeze-dryer only if it is equipped with a pipe that is properly connected to the outlet of the vacuum pump/exhaust filter (oil mist separator) and led to the outside via the roof!
- Depending on the product that is dried in the freeze-dryer, it may be necessary to install a suitable filter system in the exhaust gas pipe!
   Compliance with the local rules and regulations concerning the protection of the environment must be ensured!



Refer to the separate instruction manual of the vacuum pump and exhaust filter (oil mist separator)!

The vacuum pump must be connected to the vacuum connection of the unit and to the electrical socket at the back of the unit, which is marked accordingly (see chapter 2.1.1 - "Functional and operating elements").



#### 5 Set-up and connection



The vacuum pump is supplied with power by the unit, but the maximum current for the vacuum pump is limited. It is absolutely essential to refer to the label of the electrical outlet for the vacuum pump (see the following picture)!

If the current requirement of the vacuum pump is higher than the value that is stated on the label, the pump must be supplied separately via an on-site power socket.

 Label indicating the maximum current



Fig. 12: Indication of the maximum current for the vacuum pump (example)

The oil mist that escapes when the pump is in operation must be retained or carried off by way of an exhaust filter (oil mist separator).

- We strongly recommend using an exhaust filter (oil mist separator).
   This filter prevents air pollution by oil mist that is emitted more or less strongly by the pump depending on the working pressure.
- Use the freeze-dryer only if it is equipped with a pipe that is properly
  connected to the outlet of the oil mist separator and led to the outside
  via the roof. The hose must be laid so that the condensate cannot flow
  back into the pump. In the case of upward leading hoses, we
  recommend using a separator (Woulfe's bottle or wash bottle).



## 5.2.3.2 Dry-running vacuum pump with silencer



## Danger of poisoning/infection due to exhaust air

The exhaust air may contain harmful substances originating from the product.

Contact with particles in the exhaust air (especially by inhalation) may result in severe damage to health.

- Use a silencer with integrated filter elements or depending on the product – guide the exhaust gases from the outlet of the vacuum pump to a suitable treatment system in order to prevent the discharge of harmful substances into the surrounding atmosphere! Compliance with the national rules and regulations for the protection of the environment must be ensured!
- When working on the vacuum system (and especially on the vacuum pump), it may be necessary to wear suitable protective clothing, gloves and a breathing mask depending on the product!



Refer to the separate instruction manual of the vacuum pump and silencer!

The vacuum pump must be connected to the vacuum connection of the unit and to the electrical socket at the back of the unit, which is marked accordingly (see chapter 2.1.1 - "Functional and operating elements").



The vacuum pump is supplied with power by the unit, but the maximum current for the vacuum pump is limited. It is absolutely essential to refer to the label of the electrical outlet for the vacuum pump (see the following picture)!

If the current requirement of the vacuum pump is higher than the value that is stated on the label, the pump must be supplied separately via an on-site power socket.

1 Label indicating the maximum current



Fig. 13: Indication of the maximum current for the vacuum pump (example)



#### 5 Set-up and connection

The freeze-dryer is equipped with a dry-running vacuum pump. As a result, the vacuum exhaust gases are completely free from oil particles. However, small quantities of debris from worn seals may be emitted. That is why, even when working with non-harmful substances, the exhaust gases must either be led to the outside through the roof via a pipe that is properly connected to the outlet of the vacuum pump, or they must be filtered by way of a silencer with integrated filter elements that is connected to the outlet of the vacuum pump.

This freeze-dryer uses a silencer with integrated filter elements . The silencer is removed for transport and must be installed prior to commissioning the freeze-dryer:

- Switch the freeze-dryer off.
- Clean the vacuum connector of the freeze-dryer with a cloth.
- Fasten the silencer to the vacuum connector by way of the supplied centring ring and clamping ring.

## 5.2.4 Pressure control valve

The pressure control valve is integrated in the suction pipe between the vacuum pump and ice condenser chamber. During certain, specified process phases, it interrupts the volume flow to the vacuum pump (see chapter 2.2.1 - "General information on freeze-drying").



Observe the installation direction of the pressure control valve!

- Pressure control valve
- 2 Vacuum pump connection

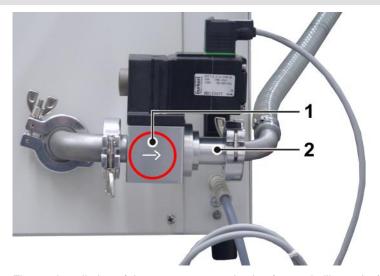


Fig. 14: Installation of the pressure control valve (example illustration)



#### 5.2.5 Vacuum sensor



Please refer to the separate operating manual of the vacuum sensor!

As standard, the freeze-dryer is equipped with a Pirani vacuum sensor (e.g. Thyracont VCP63, position see chapter 2.1.1 - "Functional and operating elements").

As a standard option, capacitive vacuum sensors (Pfeiffer CMR 363 and 364) can be retrofitted, e.g. if solvent-containing products are to be processed.



If only capacitive sensors are used, comparative pressure measurement is not possible.

#### Installation of the vacuum sensor

In order to protect the vacuum sensor against transport damage, it comes supplied in its original packaging. Prior to commissioning the freeze-dryer, the sensor must be installed.

- Switch the unit off by actuating the mains power switch.
- The screws for the left-hand side panel are located at the back of the unit. Loosen the screws and take the panel off diagonally towards the back.
- Take the vacuum sensor out of its original packaging and fasten it to the connector with a clamping ring (DIN16KF) and a centring ring (both included in the scope of supply).
- Plug the connector (installed on the unit) onto the vacuum sensor and hand-tighten the screw on the connector.



It is absolutely essential to comply with the manufacturer's instructions in the separate operating manual of the vacuum sensor!



The vacuum sensor comes supplied in a calibrated state.

After power-on, the vacuum sensor needs a few minutes to reach its operating temperature.



#### 5.2.6 Rubber valves

The rubber valves (part no. 121860) enable the connection of round-bottom flasks, wide-neck filter bottles, or distributors for ampoules to a manifold or drying chamber. Depending on the connector of the components, the blue plug can be removed.

- 1 Locking handle
- 2 Aeration connection
- 3 Vessel connection
- 4 Rubber plug
- Connection to freezedryer (e.g. via a manifold)




Fig. 15: Rubber valve



The rubber valves come supplied in an ungreased state. This is why a thin layer of vacuum grease must be applied to the connector of the freeze-dryer as well as to the vessel connector prior to start-up in order to ensure trouble-free operation.

In position A (see figure below), the aeration connector is open and the vessel connector is closed. The accessory will be aerated while the vacuum inside the drying chamber is maintained. As a result, vessels can be exchanged without any interruption of the drying process.

In position B, the aeration connector is closed and the vessel connector is open. The connected accessory is connected to the freeze-dryer.

In position C, the aeration connector and the vessel connector are closed.



Fig. 16: Possible positions of the locking handle



## 6 Operation

## 6.1 Initial start-up



Risk of injury caused by consequences of transport damage, or improper connections (e.g. escaping media).

Leaks after the transport, set-up, and connection of the freeze-dryer may lead to problems, e.g. the escape of media (depending on the configuration of the freeze-dryer, e.g. refrigerant, heat transfer medium, hydraulic oil, nitrogen, hydrogen peroxide, etc.), at a later time during the initial start-up of the freeze-dryer.

This may lead to severe damage to health or even life-threatening injuries.

 Prior to the initial start-up of the freeze-dryer, all of the supply and disposal connections must be checked for leaks by specialised persons.

## 6.2 Installation of accessories

The accessories must be completed in accordance with the drying method that is applied as well as in accordance with the scope of supply.

## 6.3 Preparation

The ice condenser chamber must be clean and dry.

- Remove any water residues from the preceding run.
- Close the aeration valve and the media drain valve.
- Ensure that all of the valves of the accessories are closed.
- Switch the vacuum pump on.

## 6.4 Switching the freeze-dryer on

Actuate the mains switch.

The control unit performs a self-test and an initialisation. This may take several seconds.

Follow the safety instructions and hazard warnings (see chapter 3 - "Safety")!



## 6.5 Loading door



## Risk of crushing caused by the movement of the loading door

Due to its relative high mass, the movement of the loading door can hardly be slowed down or stopped.

There is a risk of crushing of body parts between the door and the front of the chamber.

- Move the loading door slowly holding the door handle when opening or closing it. Do not hold the door leaf by its edge!
- Lock the door by turning the door handle!

After the drying chamber has been loaded, the loading door is closed and pressed tightly against the flange of the drying chamber with the aid of the locking handle. The locking handle is now in a perpendicular position with regard to the door edge (see figure below). When a vacuum builds up inside the drying chamber during the drying process, the loading door will be pulled closer to the flange of the drying chamber. As a result, the locking handle will be loosened and it will hang down loosely.



If the locking handle does not hang down perpendicularly when the loading door is closed, it can be readjusted. To do so, loosen the hexagon socket screw (size 8), readjust the locking handle, and retighten the screw.



Do not tighten the locking handle when there is a vacuum inside the drying chamber. During the aeration, the pressure on the locking handle will increase to such an extent that the loading door may be damaged beyond repair!

- 1 Door latch
- 2 Locking handle

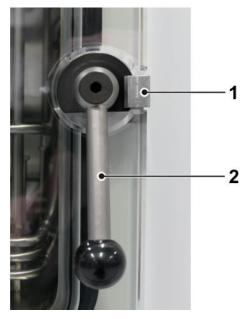


Fig. 17: Example of a door locking system of the loading door



## Radiation Shield film for loading doors made of acrylic glass

Loading doors made of acrylic glass have a special, transparent film on the exterior side of the acrylic glass door. This film reduces the transfer of radiant heat onto the product and ensures homogeneous freeze-drying results. It addition, it reduces any potential thawing effects and ensures safe and quick drying close to the freezing point.



Comply with the cleaning instructions concerning the film (see chapter 8.1.2.1 - "Lamination of the loading door with a special film")!



## 6.6 LSCplus control system

The control system LSCplus (Lyo Screen Control plus) was specifically developed for the control of freeze-drying processes. The clear user interface enables the intuitive operation of the unit.



Fig. 18: Start screen of the LSCplus control unit (example)

#### 6.6.1 User interface

The system is operated via a touch panel, i.e. by touching the buttons on the display. Every button is marked by a frame. Pressing the button activates the associated function. Depending on the function, a dialog box opens, a value can be changed, or a transaction can be confirmed.



Fig. 19: Buttons are marked by a frame



The user interface is divided into four main windows that can be called up by touching the corresponding buttons:

#### Manual

This window is also the standard user interface. It is used to control the freeze-drying process manually.

## **Program**

This area is used to create and execute programs for automating the freeze-drying process and for making it reproducible. This function is only available in combination with the programmer module PGMplus option.

#### **Options**

This window is used for personalised settings that enable the users to adapt the system as far as possible to their respective area of activity.

#### ?

In this window, the users can find all of the relevant information concerning the control system at a glance. In the event of enquiries at the factory, these data facilitate the assignment and expediting of the processing of the enquiries.

#### 6.6.1.1 Main window "Manual"

This main window shows all of the relevant process data. Here, the individual phases of a freeze-drying process can be controlled manually.

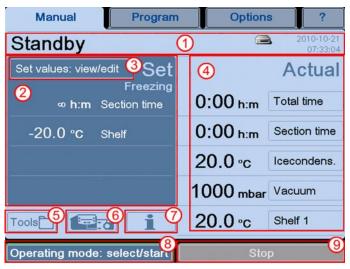


Fig. 20: Overview of the main window "Manual"

- 1 Status line
- 2 Set process values
- 3 Button "Set values: view/edit"
- 4 Actual values of the current process
- 5 Button "Tools"
- 6 Button "Schematic system diagram"
- 7 Button "Process- and equipment messages"
- 8 Button "Operating mode: select/start"
- 9 Button "Stop"



### Status line (1)

This line shows the operating status of the freeze-dryer as well as the active phase.

The status line also shows the current date and time. The clock is battery-buffered and must be reset after a failure (see chapter 6.6.1.3 - "Main window "Options"", section "Administration").

In addition, the drive symbol provides information concerning the status of the external data storage device or of the network drive. The following symbols are possible:

No symbol	No USB storage device or LAN network connected
	USB storage device connected
	Process recording on a USB storage device active
	Network available, but no network drive connected
	Network drive connected (e.g. LPCplus, LyoLogplus)
	Network drive connected and process recording active

### Set process values (2)

In the manual mode, the set values for the individual phases of the freezedrying process must be entered prior to the start of the process. Value ranges have been saved for the various phases. These value ranges can be displayed in the input window with the aid of the buttons "min" or "max" (see chapter 6.6.2.1 - "Entering set values in the manual mode").

## Button "Set values: view/edit" (3)

This button is used to call up the various parameters that can be edited.

### Actual values of the current process (4)

This area shows the current process data. The fields can be configured as desired:

Select the button of the field that is to be adapted. A dialog box opens:



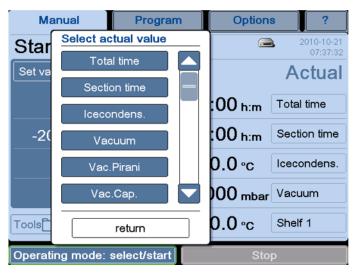


Fig. 21: Dialog box "Select actual value"

• Select the desired configuration or quit the dialog box by pressing the "return" button.

In this way, it is possible to configure a personalised overview of the actual values.

## Dialog box "Tools" (5)

This dialog box is used to call up various aids and resources.

## Vapour pressure curve above ice

A diagram shows the relationship between the pressure and sample temperature for aqueous systems. The pressure and temperature values can be changed by pressing the buttons or by moving the arrows (see figure below, item 1). The other value will be adapted automatically.

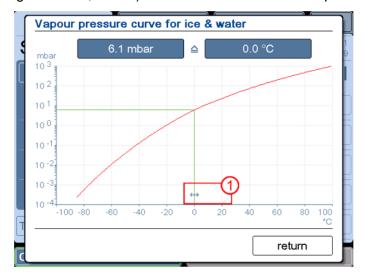


Fig. 22: Dialog box "Vapour pressure curve above ice"



#### Option: USB process recording

(see chapter 6.7 - "Optional extensions and special equipment")

- Select the "Process recording" function in the dialog box "Tools".
- Select the input fields ("Batch data"). A keyboard for the data input will be displayed.
- If necessary, select the "Options" tab, choose between manual or automatic recording, and define a recording interval.
- Press the "return" button in order to close the dialog box.

The process recording will now run in the background.



Fig. 23: Dialog box "USB process recording"

Option: Pressure increase test (only with the → double-chamber method) (see chapter 6.7 - "Optional extensions and special equipment")

The  $\rightarrow$  pressure increase test can only be performed when the freeze-dryer is equipped with an intermediate valve. The performance is possible in the manual mode as well as in the program mode, Additionally, the pressure increase test can be automatically performed as part of a program (see chapter 6.6.3.1 - "Creating a program").

- Select "Pressure increase test" in the "Tools" dialog box.
- Enter the set values for the duration and maximum pressure increase with the aid of the buttons.
- Start the pressure increase test. The test time will be displayed. After the end of the test, a status message (pressure increase was successful or failed) will be displayed together with the measured values:



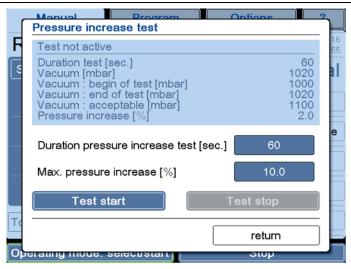


Fig. 24: Dialog box "Pressure increase test"

The "Test stop" button stops the pressure increase test.

## Option: LyoBalance weighing system

If the freeze-dryer is equipped with a LyoBalance weighing system (see chapter 6.7 - "Optional extensions and special equipment"), then the corresponding parameters must be configured in this dialog box.



Please refer to the separate operating instructions of the weighing system!

#### Dialog box "Schematic system diagram" (6)

Pressing the button "Schematic system diagram" displays a schematic diagram of the system on the left-hand side of the screen, including all the components. Active components are displayed in green. Touching a component calls up its name and  $\rightarrow$  reference designator.



Fig. 25: Schematic system diagram with the name and reference designator of the component



## Dialog box "Process and equipment messages" (7)

This dialog box shows and saves all of the error messages and other messages. In the event of an error or message, the window "Process and equipment messages" will open automatically. In addition, a sound signal is emitted until the error is acknowledged.

Malfunctions are divided into three categories:

Red: error messagesOrange: process messagesYellow: general messages

The representation of the message provides information on its current status. A double frame around a message means that the error has not been eliminated yet. The colour of the button "quit" changes from blue to grey once the message has been acknowledged.



Fig. 26: Representation of an error message

The advantage of this system is that malfunctions that occurred during the night can be discovered the next day even if the cause of the malfunction has already been eliminated.

The dialog box cannot be quit until all of the messages have been acknowledged.

If a message has been acknowledged although the malfunction has not been eliminated, the button "Process and equipment messages" will be displayed in the respective colour of the malfunction in the main window.

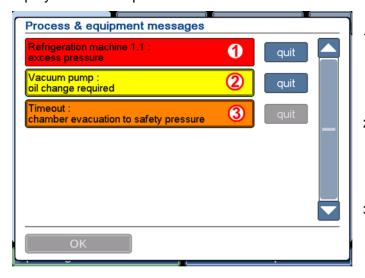


Fig. 27: Dialog box "Process and equipment messages"

- The malfunction has been eliminated, but the message has not been acknowledged
- 2 The malfunction has not be eliminated and the message has not been acknowledged yet
- The malfunction has not been eliminated yet, but the message has been acknowledged



#### **Details**


Touching the message calls up details concerning the error message:

- · Cause of the message,
- Effects of the message,
- Measures to eliminate the error,
- → Reference designator,
- Error counter (indicates how often this error has occurred) and the time stamp of the last error message.

Use the arrow keys to call up the individual windows.



The error message text is always followed by an error code. Always indicate the error code in the event of enquiries or service requests!

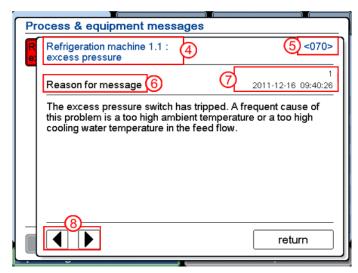

- 4 Error message
- 5 Error code
- 6 Detailed information
- 7 Error counter and time stamp of the last error
- 8 Arrow keys

Fig. 28: Details concerning an error message



The texts of the process and error messages are not included in this operating manual.

You can order these documents from our service department.



## Dialog box "Operating mode: select/start" (8)

After the set values have been entered for the process, the process can be started manually with this function (see chapter 6.6.2 - "Manual freezedrying").



Fig. 29: Dialog box "Operating mode: select/start" (The version of the dialog box that is displayed depends on the equipment of the freeze-dryer.)

#### Button "Standard unit test"

Apart from the process phases of the freeze-drying process ("Freezing", "Warm-up", "Main drying", and "Final drying") and the operating mode "Defrosting", the button "Standard unit test" is also available. This button opens a selection of various tests with fixed parameters. After consultation with the manufacturer, these tests can be performed in order to check the functionality and processes of the freeze-dryer.



Some of the available tests are also provided in the form of program templates (see chapter 6.6.3.1 - "Creating a program").

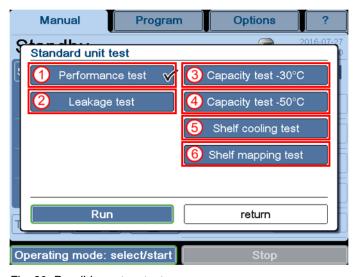


Fig. 30: Possible system tests



## Performance test (1)

The performance test is used to determine the following performance parameters:

- vacuum decrease rate
- final vacuum
- · minimum ice condenser temperature
- shelf cooling rate
- minimum shelf temperature
- · shelf heating rate



Prior to performing a test, ensure that the chamber is dry and unloaded.

#### Procedure:

- In the main window "Manual", select the button "Operating mode: select/start" "Standard unit test".
- Select "Performance Test" and start the test via the "Run" button.

The test will be performed. The parameters will be measured at defined points of time, evaluated, and displayed in a dialog box (see the following illustration).

If the freeze-dryer is equipped with the LPCplus SCADA software, the results will be documented in the event list.

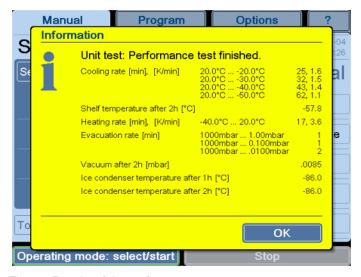


Fig. 31: Results of the performance test

#### Evaluation:

Please contact the Christ support team for the evaluation of the test run.

## Leakage test (2)

The leakage test enables the chamber of the freeze-dryer to be tested for tightness in view of any gaseous or liquid media. Since absolutely tight components simply do not exist, a leak rate is determined.



#### Procedure:

- In the main window "Manual", open the dialog box "Set values: view/edit" via the corresponding button and then select the button "Leakage test".
- Edit the values "Duration test" (value between 10 min and 18 h) and "Chamber volume" (value see technical data), confirm the new values and return to the main window.
- In the main window "Manual", select the button "Operating mode: select/start" "Standard unit test".
- Select "Leakage test" and start the test via the "Run" button.

The parameters for the leakage test have been developed by Martin Christ Gefriertrocknungsanlagen specifically for freeze-dryers. In a first step, these parameters (vacuum, ice condenser temperature) must be reached. It is not until the conditions are fulfilled that the pressure control valve closes. Then, the actual leakage test is performed in a second step.

The result will be indicated by way of a dialog box.

If the freeze-dryer is equipped with the LPCplus SCADA software, the results will be documented in the event list.

#### Evaluation:

The leakage rate that is calculated after the test provides information concerning the tightness of the system. If the threshold value is not reached, the test has been passed. If it is exceeded, the test has been failed.

#### Capacity test -30°C (3)



The capacity test -30°C is intended for units with one single-stage and one double-stage refrigeration system.

The capacity test -30°C is a freeze-drying program/ for verifying the ice condenser capacity (when the shelves are cooled to -30°C in the "Freezing" phase). For this purpose, the shelves must be loaded.

#### Procedure:

- Load the shelves evenly with water in dishes for the test. The water quantity must be 2/3 of the maximum ice condenser capacity that is specified for the freeze-dryer.
- In the main window "Manual", select the button "Operating mode: select/start" – "Standard unit test".
- Select "Capacity test -30°C" and start the program via the "Run" button.

In the "Freezing" phase, the shelves are cooled to -30°C. The parameters for the subsequent "Main drying" and "Secondary drying" sections have been configured in such a way that the water will be completely sublimated out of the dishes and bound on the ice condenser after 24 hours.



At the end of the process, a pop-up window with a safety enquiry (confirmation prompt) opens. Following the confirmation of this enquiry, the freeze-dryer will be switched to standby.

#### Evaluation:

The test is passed if the dishes do not contain any water/ice after the end of the process.

Capacity test -50°C (4)



The capacity test -50°C is intended for units with a minimum of two double-stage refrigeration systems.

The capacity test -50°C is a freeze-drying program/ for verifying the ice condenser capacity (when the shelves are cooled to -50°C in the "Freezing" phase). For this purpose, the shelves must be loaded.

#### Procedure:

- Load the shelves evenly with water in dishes for the test. The water quantity must be 2/3 of the maximum ice condenser capacity that is specified for the freeze-dryer.
- In the main window "Manual", select the button "Operating mode: select/start" "Standard unit test".
- Select "Capacity test -50°C" and start the program via the "Run" button.

In the "Freezing" phase, the shelves are cooled to -50°C. The parameters for the subsequent "Main drying" and "Secondary drying" sections have been configured in such a way that the water will be completely sublimated out of the dishes and bound on the ice condenser after 24 hours.

At the end of the process, a pop-up window with a safety enquiry (confirmation prompt) opens. Following the confirmation of this enquiry, the freeze-dryer will be switched to standby.

#### **Evaluation:**

The test is passed if the dishes do not contain any water/ice after the end of the process.

#### **6 Operation**



## Shelf cooling test (5)



The test is intended solely for freeze-dryers of the type Epsilon 2-6D LSCplus and Epsilon 2-10D LSCplus.

The shelf cooling test is used to check the performance of the shelf cooling system (refrigeration unit 2) during the "Main drying" phase.

The shelves must be empty for the test.

#### Procedure:

- In the main window "Manual", select the button "Operating mode: select/start" – "Standard unit test".
- Select "Shelf cooling test" and start the test via the "Run" button.

The parameters for the "Main drying" sections have been configured in such a way that refrigeration system 1 only acts on the ice condenser, whereas the shelves are cooled solely by refrigeration system 2.

At the end of the process, a pop-up window with a safety enquiry (confirmation prompt) opens. Following the confirmation of this enquiry, the freeze-dryer will be switched to standby.

#### Evaluation:

Please contact the Christ support team for the evaluation of the test run.

#### Shelf mapping test (6)

The shelf mapping test is a freeze-drying program for bringing the shelves to a temperature of +20°C, -40°C, and +40°C for a specific period of time in order to be able to determine the temperature distribution on the shelves for each of these three temperatures with the aid of an external shelf mapping system.

The thermoblocks of the shelf mapping system with the inserted temperature sensors must be distributed evenly on the shelves and connected to the external measurement recorder for the test.

#### Procedure:

- In the main window "Manual", select the button "Operating mode: select/start" "Standard unit test".
- Select "Shelf mapping test" and start the program via the "Run" button.
- Start the external measurement recording process at the same time.

During the test, the predefined shelf temperature values are adjusted and maintained constant for a specific period of time in order to keep the temperature distribution in a static state.





At the end of the process, a pop-up window with a safety enquiry (confirmation prompt) opens. Following the confirmation of this enquiry, the freeze-dryer will be switched to standby.

The external measurement recording process can then be stopped.

#### **Evaluation:**

Please contact the Christ support team for the evaluation of the test run.


## Button "Stop" (9)

Pressing this button stops the current process. The system switches to the standby status.



## 6.6.1.2 Main window "Program"

In the main window "Program", pre-programmed freeze-drying processes can be loaded and edited and new programs can be created with the PGMplus programmer module.

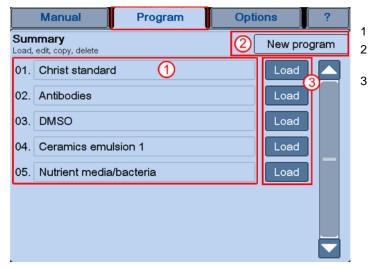

Buttons "Load"

program"

Program list

Button "New

Fig. 32: Overview of the main window "Program"

#### **Program list (1)**

After the selection of the main window "Program", an overview of the programs that have already been saved will be displayed. Pressing the button "Load" (3) behind the program name calls up the program data. Programs can be loaded, edited, copied, or deleted (see chapter 6.6.3 - "Freeze-drying with the PGMplus programmer module ").

## "Dialog box "New program (2)

In this dialog box, new programs can be created either based on an already existing program or completely from scratch (see chapter 6.6.3.1 - "Creating a program").



## 6.6.1.3 Main window "Options"

The main window "Options" is used to perform fundamental basic settings of the control system in order to adapt it perfectly to the respective area of application of the freeze-dryer.

### General

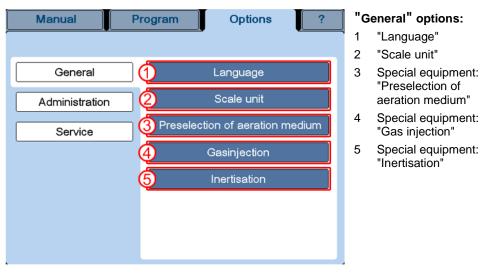


Fig. 33: Overview of the main window "Options/General"

## Language (1)

The control system can be used in several languages which can be selected via the dialog box.



Fig. 34: Dialog box "Change language"



## Change scale unit (2)

This dialog box is used to change the unit of measurement for the temperature and vacuum.

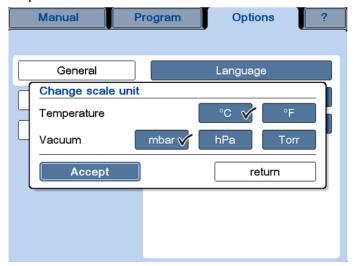


Fig. 35: Dialog box "Change scale unit"

#### Special equipment: Preselection of the aeration medium (3)

This function can be performed in the manual mode or saved together with a program (see chapter 6.6.3.1 - "Creating a program").

If the freeze-dryer is equipped with an automatic aeration valve and automatic valves for media selection, this dialog box can be used to preselect the medium that is to be used for all of the aeration medium requests in the manual mode (as of the start of the main drying phase) and during the "Aeration" section. The phases "Freezing" and "Warm-up" in the manual mode and the operating modes "Defrosting", "Leakage test", and "Media drain" always use air for aeration.

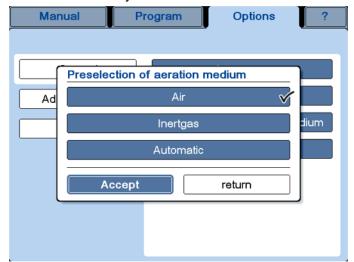


Fig. 36: Dialog box "Preselection of aeration medium"

If the vacuum control system of the freeze-dryer uses a controlled gas inflow (gas injection, bleeding), the preselected medium will be used for this purpose.



The following media preselection settings are possible:

- Air: Preselects the media connection "Air".
- Inert gas: Preselects the media connection "Inert Gas".
- Automatic: Automatic media connection preselection depending on the chamber pressure and stoppering status of the product vials:
  - Chamber pressure ≥ 950 mbar: Preselection of the media connection "Air".
  - Chamber pressure < 950 mbar: Preselection of the media connection "Inert gas".

#### Special equipment: Gas injection with a proportional valve (4)

This function can be performed in the manual mode or saved together with a program (see chapter 6.6.3.1 - "Creating a program").

If the freeze-dryer is equipped with a proportional gas injection valve, the dialog box "Gas injection" can be used to preselect the vacuum control method that is to be used.



Fig. 37: Dialog box "Gas injection"

The following methods are possible:

- Button "Off": The gas injection is deactivated. Vacuum control is ensured solely by opening and closing the pressure control valve in the suction line of the vacuum pump.
- Button "Standard": Vacuum control is ensured by combined evacuation and gas injection. The gas injection solenoid valve that is installed in series with the proportional valve is continuously open. If the actual vacuum is better than the set value, gas will be injected by opening the proportional valve. The opening width of the valve is automatically controlled. If it is worse than the set value, evacuation will be performed by opening the pressure control valve in the suction line of the vacuum pump.
- Button "Continuous": In the range between 6 mbar and the final vacuum, vacuum control is performed with the pressure control valve and the gas injection solenoid valve being continuously open and solely by varying the injection flow with the aid of the proportional valve.
   Initially, the proportional valve is closed. Above 6 mbar, the vacuum is controlled using the "Off" method.



## Special equipment: Inertisation (5)

(see chapter 6.7 - "Optional extensions and special equipment")

If the "Inertisation" option is active and the freeze-dryer is in the "Standby", "Manual - Freezing", "Program - Loading" or "Program - Freezing" mode, the automatic inertisation of the drying chamber will be performed for the preselected inertisation time after the loading door has been closed. The operating mode then switches to "Run Inertisation".



Fig. 38: Dialog box "Inertisation"

A successful inertisation is a prerequisite for continuing the various processes in the following operating modes:

- Manual
- Program
- Defrosting
- Media drain.

All other operating modes can be started without successfully completing the inerting sequence.

The following parameters can be set:

- The inertisation time determines the effective inertisation duration with open inlet and outlet valves and can be set in a range of 1...9999 seconds.
- The parameter "Delay on" determines the duration from the opening of the inlet valves to the opening of the outlet valves. The setting range is 0...99 seconds.
- The parameter "Delay off" determines the duration from the closing of the inlet valves to the closing of the outlet valves. The setting range is 0...99 seconds.

An inertisation process can be stopped any time by pressing the "Stop" button.



If the inertisation has been started in the "Manual - Freezing", "Program - Loading" or "Program - Freezing" mode, the "Stop" button will also abort the freeze-drying process!



If the volume flow through the inertisation line falls below a certain threshold for more than 5 seconds (the value can be preset at the flow meter) or if the loading door is opened during an inertisation sequence, the process will also be aborted immediately.



In order to prevent unauthorised access to the "Inertisation" dialog box, we recommend protecting the access to the control system by way of a password (see chapter 6.6.1.3 - "Main window "Options"", section: "Administration"/"Access protection " (4)).

#### Administration

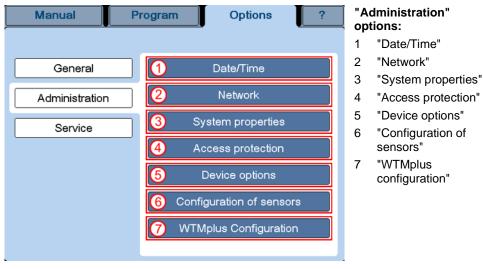


Fig. 39: Dialog box "Options/Administration"

## Date/Time (1)

The LSCplus control system is equipped with an integrated, battery-buffered clock. After a failure of the buffer battery, the date and time must be reset.

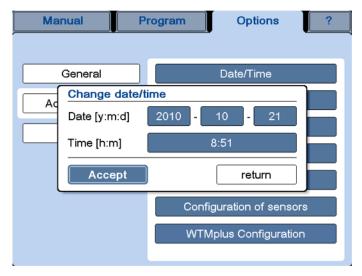


Fig. 40: Dialog box "Change date/time

#### 6 Operation



#### Network (2)

This dialog box is used to change various system settings.



The modifications will not become effective until after a restart of the unit.

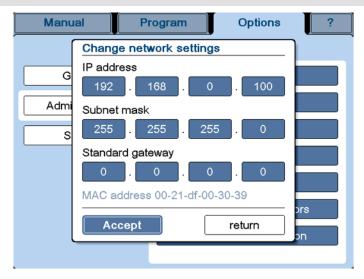


Fig. 41: Dialog box "Network"

## System properties (3)

This dialog box is used to change various system settings.

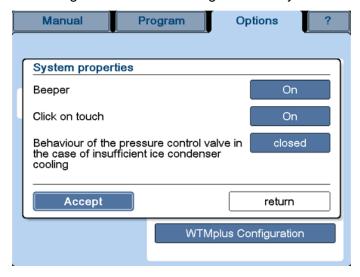


Fig. 42: Dialog box "System properties"

Beeper: The beeper sounds in the event of a malfunction, for example.

- If the setting is "On", the beeper sounds every few seconds until the user acknowledges the message.
- If the setting is "Silent", the beeper sounds once when the malfunction occurs.
- If the setting is "Off", the beeper will not sound at all.



*Click on touch:* If this function is active, a clicking sound can be heard whenever the system registers that a button has been touched.

Behaviour of the pressure control valve in the case of insufficient ice condenser cooling: If this function is active (button "closed"), the pressure control valve will close at an ice condenser temperature of ≥ -20°C during the drying process in order to avoid damage to the vacuum pump caused by the withdrawal of condensable gases. A corresponding error message will be displayed. Pressing the button again deactivates the function (button "controlled").

## Access protection (4)

In this dialog box, the access rights can be managed on several levels and they can be protected with a password.

In the factory setting with an activated access protection, data can be viewed but not edited.

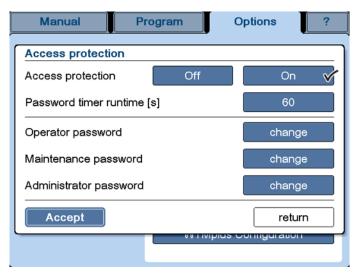


Fig. 43: Dialog box "Access protection"



The other buttons cannot be activated unless the access protection is active.

Password timer runtime: In order to prevent unauthorised access, the system will automatically switch back to the default setting after a predefined period of time.

In this case, there is a small lock symbol in the status line and below this symbol the remaining time until the lock will be active is counted down. At the same time a button with a big lock symbol will be displayed in the actual values field.



Fig. 44: Countdown of the password timer and the button with the lock symbol



 The button with the lock symbol blocks the access immediately and the system switches to the default setting.



Fig. 45: Access blocked, the data cannot be edited

Operator/maintenance/administrator password: For each of these access levels, certain editing rights have been defined. They can be enabled with the corresponding password.

The rights of the various access levels are detailed in the following table.

Action	Operator	Maintenance	Administrator
Editing of the data of the current process run (e.g. selection of the operating mode, changing of set values)	✓	✓	<b>√</b>
Editing of maintenance functions (e.g. oil change of the vacuum pump)		<b>✓</b>	<b>✓</b>
Editing of the default settings (e.g. editing of the access protection, creating and editing of programs, editing of system settings)			<b>√</b>

#### Device options (5)

This dialog box lists all of the device options that are available for the unit in question. A list of all the possible options can be found at chapter chapter 6.7 - "Optional extensions and special equipment". Options that require a series-number-specific release code are marked with the symbol ("6").

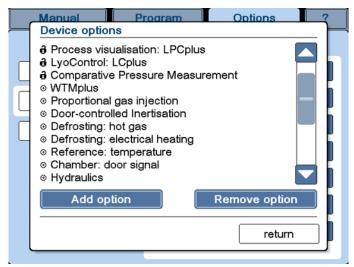


Fig. 46: Dialog box "Device options" (example)



If the freeze-dryer is to be extended by an option, this option must be enabled via this dialog box.

- Press the button "Add option". An input window opens.
- Enter the six-digit Christ activation code that was supplied for this option. Note that the keys are case sensitive.

Options can be removed in the same way.



The modifications will not become effective until after a restart of the unit.

#### Configuration of sensors (6)



The sensor configurations depend on the equipment version of the unit. If the configuration is incorrect, the correct operation of the unit cannot be quaranteed.

This dialog box is used for the configuration of the existing sensors.

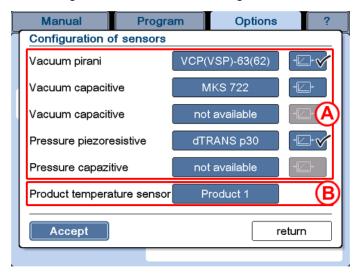


Fig. 47: Dialog box "Configuration of sensors" (example

Vacuum sensors (see the illustration above, item A)

For the vacuum as well as pressure, there are two different measuring methods, and for each of these methods, different sensors can be selected.

• In order to change the sensor, press the button with the sensor name. The possible models will be displayed one after the other.

The buttons on the right-hand side of the sensors show a control symbol. The tick marks on the buttons indicate the control sensors, i.e. the sensors that are decisive for the vacuum inside the unit. If there is a second sensor, the data of this sensor are simply used for comparison.



Product temperature sensor (see the illustration above, item B) Only for systems with a WTMplus system

The wired product temperature sensor 1 is the default sensor for determining the value " $\Delta T$  product" (see chapter 6.6.3 - " Freeze-drying with the PGMplus programmer module ", section "Conditions for switching to the next section").

If the freeze-dryer is equipped with a wireless WTMplus temperature measurement system, it is also possible to select a different wired product temperature sensor or a WTMplus sensor:

- Select the button of the product temperature sensor. A drop-down menu showing the available sensors opens.
- Select the sensor that you would like to use for determining "ΔT product".
- Exit the drop-down menu. Select the button "Accept" to close the dialogue box and to save the selection.



Fig. 48: Selection of the product temperature sensor (only for systems with a WTMplus system)



## WTMplus configuration (7)



The dialog box is displayed for information purposes only.

The configuration can be changed only via the LPCplus user interface.

This dialog box shows all of the existing WTMplus sensors. Every sensor is assigned to a measuring channel based on its serial number. Next to the Number of the measuring channel and the serial number of the sensor, the associated temperature and a signal quality index (SQI) are displayed. A bar in the fields indicates the signal quality:

Green: good signal qualityYellow: medium signal qualityRed: insufficient signal

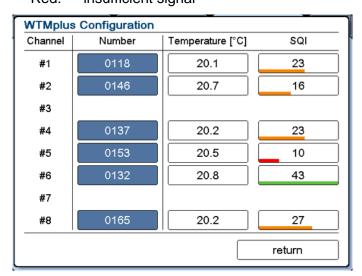


Fig. 49: Dialog box "WTMplus configuration"



#### **Maintenance**

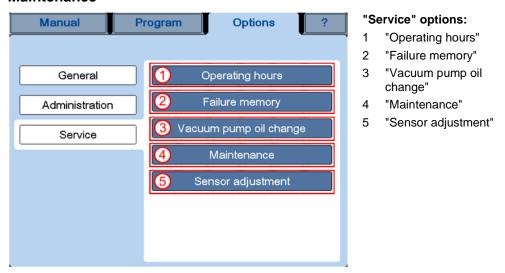


Fig. 50: Dialog box "Service" (varies depending on the type of system)

## Operating hours (1)

This dialog box is used to call up the number of operating hours of the various components of the freeze-dryer, e.g. the refrigeration unit, vacuum pump, or pressure control valve. In addition to the name, the  $\rightarrow$  reference designator is also displayed.

These data are provided for the purpose of information only. They cannot be edited.

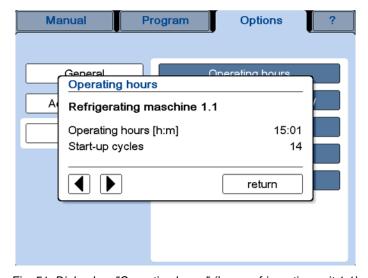


Fig. 51: Dialog box "Operating hours" (here: refrigeration unit 1.1)



#### Failure memory (2)

Equipment information system. These messages can be viewed in this dialog box. The failure memory includes the last 32 messages. If this number is exceeded, the oldest message will be overwritten.

Use the arrow keys to call up the individual messages.

The error message text is always followed by an error code.



Always indicate the error code in the event of enquiries or service requests!

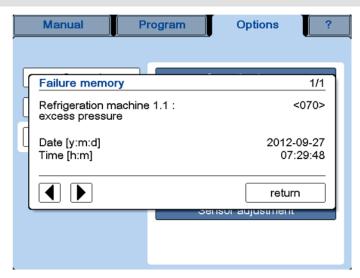


Fig. 52: Dialog box "Failure memory"





#### Vacuum pump oil change (3)



This option only applies to oil-sealed vacuum pumps!

The system monitors the oil change interval of the vacuum pump. The interval can be adapted to the vacuum pump model and utilisation. When the end of an oil change interval is reached, a corresponding message will be displayed.

- Acknowledge the message.
- Change the oil of the vacuum pump.
- Reset the operating hour counter in the dialog box "Vacuum pump oil change" by pressing the "reset" button.

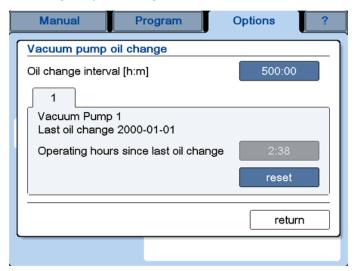


Fig. 53: Dialog box "Vacuum pump oil change"



#### Maintenance (4)

The maintenance interval of the unit is fixed at 3,000 operating hours or at least one maintenance per year.

When the end of a maintenance interval is reached, a corresponding message will be displayed.

- Acknowledge the message.
- Make an appointment for the maintenance of your freeze-dryer.
- After the maintenance, our service engineer will reset the operating hour counter in the dialog box "Maintenance".

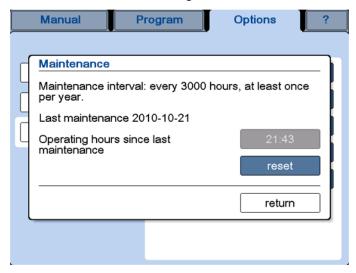


Fig. 54: Dialog box "Maintenance"

#### Sensor adjustment (5)

In this dialog box, the sensors are adjusted in terms of a predefined reference value.



Misadjusted sensors will lead to incorrect measurement values, which in turn will have a negative effect on the process control.



The sensor adjustment must be carried out by authorised specialist personnel.



#### 6.6.1.4 Main window "?"

This main window includes the most important information concerning your freeze-dryer:



Fig. 55: Freeze-dryer system information

- 1 Freeze-dryer type
- 2 Control system type
- 3 Serial number
- 4 Manufacturer contact data
- 5 Details concerning the software version



In the event of enquiries at the manufacturer, please state the number that is stated here.

#### 6.6.2 Manual freeze-drying

In the manual mode, the user switches manually from one freeze-drying phase to the next. The manual mode is activated by calling up the main window "Manual".

The set values for the individual process phases (freezing, warm-up, main drying, and final drying) are defined prior to the start of the process. Then, the freeze-drying process can be started via the dialog box "Operating mode: select/start".



If the freeze-drying process is to be started directly with the "main drying" (sublimation) phase, the vacuum pump must be warmed up approximately 15 minutes prior to the process start. Failure to do so will result in a corresponding warning message when the process starts.



If " $\infty$ " (infinite) has been preselected for a phase, the next phase must be selected manually by way of the button "Operating mode: select/start".

In the manual mode, the set values of the active phase can be changed during the process run. In this case, the control system adapts the unit to the new set values as quickly as possible.



After the completion of a phase, the system switches to the next phase without switching the unit to standby. The transition from "freezing" to "warm-up" takes place automatically. After the completion of the warm-up phase, this dialog box will be displayed:

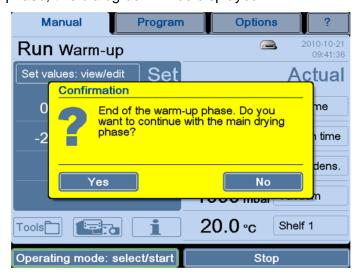


Fig. 56: Dialog box after the completion of the warm-up phase

The unit will remain in the warm-up phase until you confirm.

The transition from "main drying" to "final drying" again takes place automatically. After the completion of the "final drying" phase, the system displays another enquiry with which the freeze-drying process will be terminated. The unit remains in the "run" mode until the enquiry is confirmed.

The process can be stopped any time by pressing the "Stop" button. In this case, the unit will be switched to standby.

## 6.6.2.1 Entering set values in the manual mode

The system has stored set values for every phase, and for every value there are pre-defined value ranges that can be determined in the various dialog boxes by pressing the buttons "min" and "max".

In order to protect the product,  $a \rightarrow safety\ pressure$  value can be entered in every drying section.



#### Viewing or editing the set values:

• Press the button "Set values: view/edit" (see chapter 6.6.1.1 - "Main window "Manual""). The following dialog box will be displayed:



Fig. 57: Dialog box "Set values: view/edit"

- 1 "Aeration" button
- 2 "Defrosting" button
  - "Media drain" button (special equipment)
  - "Leakage test" button

Fields that are displayed in the form of buttons can be edited.

- Aeration (1)
  If the freeze-dryer is equipped with an automatic aeration valve, this button is used to define the aeration pressure.
- Defrosting (2)
   This button is used to pre-define the defrosting time and temperature (not for hot-water defrosting). In addition, this button is used to define whether the operating mode "media drain" (see below) will be started automatically after the defrosting process.
- Media drain (3)
  If the freeze-dryer is equipped with an automatic media drain for
  condensate water or another medium, the opening time of the drain
  valve can be pre-selected in this dialog box.
- Leakage test (4)
   This button displays the parameters that are used for the leakage test.
   In addition, the test time and the chamber volume must be stated (depending on the accessories that are used).



Setvalues: view/edit Section time freezing Freezi 1 h:m Section time 2)+/h:m Shelf œ Vacuum 2 3 mbar Safety press. 4 5 6 mbar 7 8 9 Aeration 0 Leakage test Accept return Accept

#### Numerical values can be edited with the aid of a numerical keypad:

- 1 Set value display
- 2 Button for changing the sign (e.g. when entering temperature values)
- 3 "∞" (infinite)
- 4 Button for editing the value in pre-defined steps
- 5 Selection of a possible maximum or minimum value
  - Input of a value via the numerical keypad
- 7 Button for deleting the displayed value

Fig. 58: Editing set values

- Confirm the new value and quit the numerical keypad by pressing the button "Accept".
- Confirm the input and quit the dialog box via the button "Accept".
- If the dialog box is closed by the button "return", the changes will be discarded.

## 6.6.3 Freeze-drying with the PGMplus programmer module

Unlike in the manual mode, an entire freeze-drying process can be executed fully automatically and under reproducible conditions with the aid of the PGMplus programmer module.

Freeze-drying programs are divided into sections (1). Every section in the program has certain set values (2). A program must include a minimum of two sections, and the maximum number of possible sections is 64. 32 program storage locations are available.

In every program, the system always displays four consecutive sections in order to show their connection.



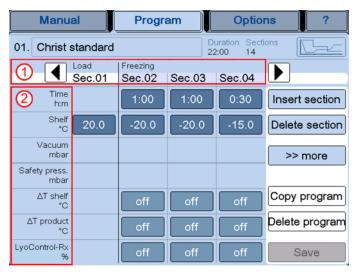


Fig. 59: Representation of a freeze-drying program

#### **Program sections**

When the programmer module executes a freeze-drying process, it executes the various sections that were created one after the other until the last section is completed.

Within the various sections, the system calculates linear ramps for the temperature and vacuum. These ramps start with the set value of the previous section and end with the set value of the current section.

As a result, there is not abrupt change of the set value from section to section, but a steady adaptation.

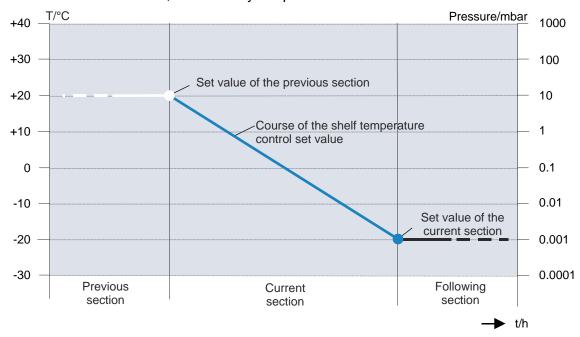


Fig. 60: Graphical representation of the course of the control set value

In order to protect the product,  $a \rightarrow safety\ pressure\ value\ can be entered in every drying section.$ 



#### Conditions for switching to the next section

For all of the program sections to be executed automatically, certain switching conditions must be fulfilled at the end of each section. If these conditions are not fulfilled, e.g. due to incorrect set values, a corresponding process message will be displayed and the section will be extended.

<u>Ice condenser temperature</u>: This value is checked only when the system switches from freezing (loading) to drying. The ice condenser temperature must be  $\leq$  -40°C.

<u>Vacuum</u>: This value is checked only during the drying phase. The actual vacuum can differ from the set value by 20% maximum. In the case of a set value of 0.001 mbar (final vacuum), there will be no check. In order to reach the vacuum as quickly as possible, a section time of 1 minute can be preselected. Since this is not possible in practice, a process message will be issued for the first time after 15 minutes in this case.

 $\Delta T$  shelf: This value defines the permissible deviation of the shelf temperature from the set value. At the end of the section, the actual temperature of the shelves (in the case of WST shelf 1) will be compared to the set value. If the shelf temperature is beyond the permissible range, the section will be extended until the deviation is within the permissible range.

<u>AT product</u>: This value defines the permissible deviation of the product temperature from the set value. By default, the wired product temperature sensor 1 is used. If the freeze-dryer is equipped with the wireless WTMplus temperature measurement system, it is also possible to select a different wired product temperature sensor or a WTMplus sensor (see chapter 6.6.1.3 - "Main window "Options"", section "Administration"/"Sensor configuration").

During the freezing phase, the product temperature may exceed the set value by the defined value. In the drying phase, the system will provide a signal to the user if the actual value lies below the set value by more than the permissible deviation.

<u>LyoControl-Rx</u> (option with <u>LyoControl LCplus</u>): The value LyoRx defines the minimum permissible value of the LyoControl sensor (measured by the LyoControl sensor 1) during the drying phase. If the actual value falls below this limit, the shelf heater will be switched off in order to prevent the product from thawing due to excessive energy input by the shelf temperature control system. The LyoControl value is checked only during the main and final drying phases.

Pressure increase test (option): Depending on the selected mode, the pressure increase test can also be used as a condition for switching to the next section (see chapter 6.6.3.1 - "Creating a program", option: pressure increase test). In the last drying section, two pressure increase tests will be performed and evaluated. If both values are not greater than the specified "pressure increase" parameter, the condition for switching to the next section is fulfilled. If this is not the case, the section will be extended. If the actual value exceeds the set value before the preselected time has elapsed, the test will be aborted in order to prevent the product from thawing.



<u>AT comparative (option)</u>: This value indicates the difference between a Pirani sensor and a capacitive vacuum sensor in per cent based on the actual value of the capacitive vacuum sensor. When the sublimation rate decreases, the difference decreases as well. As a result, the value is an indicator for determining the drying end of the main draining phase. If the set value is not reached by the end of the main drying phase, the section will be extended.



If only capacitive sensors are permissible (e.g. for freeze-drying solvent-containing products), comparative pressure measurement is not possible.

#### Vacuum pump warm-up

Apart from the execution of the various sections, the PGMplus programmer module also controls other tasks that need to be performed during the process run, e.g. the automatic activation of the vacuum pump.

If the pressure control valve is closed, the PGMplus programmer module shifts the warm-up phase of the vacuum pump to the freezing phase so that it is **before** the first drying section. Since the pressure control valve remains closed during the warm-up of the vacuum pump, neither the freezing phase nor the pressure inside the drying chamber will be affected.

The duration of the warm-up phase can be specified separately for every program (see chapter 6.6.3.1 - "Creating a program").

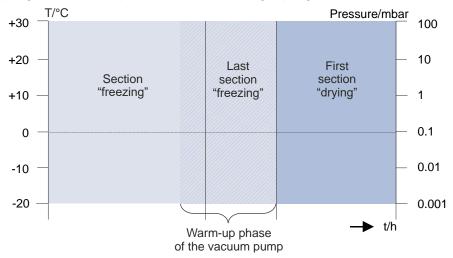



Fig. 61: The warm-up phase of the vacuum pump is shifted to the freezing phase prior to the first drying section



### 6.6.3.1 Creating a program

To create a new program:

Press the button "New program" in the main window "Program". The
dialog box that is displayed offers various different program templates.
The scroll bar on the right-hand side can be used to scroll through the
list.

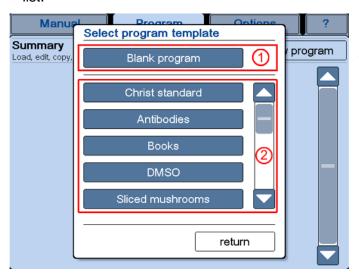

- Button for creating a blank program
- Scroll bar for selecting a program template

Fig. 62: Dialog box "Select program template"

## Creating a blank program (1)

This button is used to call up a blank program template. Only section 1 is pre-defined as the loading section. In this phase, the start conditions of the programs are defined. The room temperature (20°C) is the standard default.



If the product is frozen outside the freeze-dryer ( $\rightarrow$  double-chamber method), the shelf temperature must be adapted accordingly in section 1.

For all the other sections, the set values must be defined (see figure below):

- Press the button "Insert section" (4) and select the position of the section as well as the freeze-drying phase. The section will be inserted at the defined position.
- Adapt the parameters of the inserted section. All of the values are not available in all of the freeze-drying phases.
- Insert and edit the next section.



During the creation of a program, the order of the individual freeze-drying phases must be maintained. This means that it is not possible to insert a freezing section after a main drying section.

#### 6 Operation

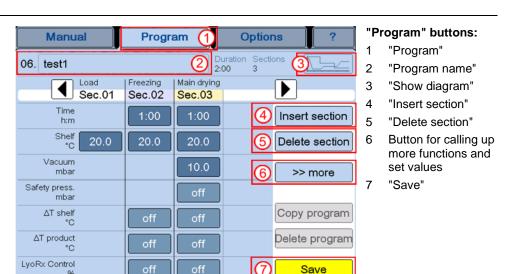


Fig. 63: Editing a blank program template

- The button "Delete section" (5) can be used to delete sections.
- The button ">>more" (6) can be used to enter more functions and set values in a program-related manner, depending on the type of freeze-dryer (see the sections below).
- Proceed in this manner in order to create an entire program according to your specific needs.
- Pressing the button "Diagram" (3) displays the program in the form of a diagram.
- Pressing the button "Program name" (2) calls up an input field in which the name of the program can be changed.
- The button "Save" (7) can be used in between or at the end of the program creation in order to save the program.
- The button "Program" (1) calls up the main window. The system will ask the user whether the program shall be saved if this has not been done yet.

The program will be automatically assigned to the first free program storage location. The creation of the program is now complete and it can be loaded.



#### Button ">>more"

The button ">>more" can be used to enter more functions and set values in a program-related manner.

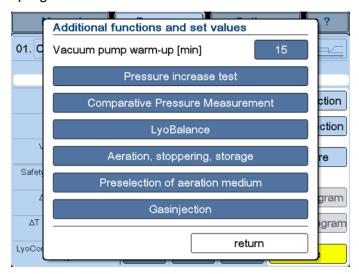


Fig. 64: Selection of program-related functions and set values

#### Vacuum pump warm-up

see chapter 6.6.3 - " Freeze-drying with the PGMplus programmer module "

Option: Pressure increase test (only with the  $\rightarrow$  double-chamber method) The  $\rightarrow$  pressure increase test can only be performed when the freeze-dryer is equipped with an intermediate valve.



The indication of the measurement value "dp Test" can be configured in chapter 6.6.1.1 - "Main window "Manual"" under "Actual values of the current process" in the dialog box "Select actual value".

In contrast to the pressure increase test in the manual mode, repeated pressing of the button in the program mode enables the selection of different variants.

- Periodic pressure increase test:
  - The test will be performed periodically during the entire main or final drying phase. The parameters "Duration test" and "Time between tests" apply. The maximum pressure increase is limited to 100%, referring to the actual value at the beginning of the measurement. If the value is exceeded, the pressure increase test will be aborted in order to prevent the product from thawing.
- Progress condition:
  - In the last main drying or final drying section, two pressure increase tests will be performed and evaluated. The start point will be calculated automatically by the control system. The parameters "Duration test" and "Time between tests" apply.
  - If, during both tests, the values of the pressure increase test are not greater than the preset "Pressure increase" parameter, the drying process will be considered complete at the current shelf temperature and chamber vacuum. Thus, the progress condition for switching to the



next section is fulfilled and the next section will be initiated. If the condition for switching to the next section is not fulfilled, a process message will be issued, the current section will be extended, and further pressure increase tests will be executed periodically until the condition is fulfilled. If the actual value exceeds the set value before the preselected time has elapsed, the test will be aborted in order to prevent the product from thawing.

#### · Periodic & progress condition:

This variant is a combination of the possibilities that are described above. The test will be performed periodically during the entire main or final drying phase. The maximum pressure increase is limited to 100%, referring to the actual value at the beginning of the measurement. If the actual value exceeds the set value before the preselected time has elapsed, the test will be aborted in order to prevent the product from thawing.

If, during both tests, the values of the pressure increase test are not greater than the preset "Pressure increase" parameter, the drying process will be considered complete at the current shelf temperature and chamber vacuum. Thus, the progress condition for switching to the next section is fulfilled and the next section will be initiated. If the condition for switching to the next section is not fulfilled, a process message will be issued, the current section will be extended, and further pressure increase tests will be executed periodically until the condition is fulfilled.

#### Disabled:

No pressure increase test will be executed during the main or final drying phase. There will be no evaluation.

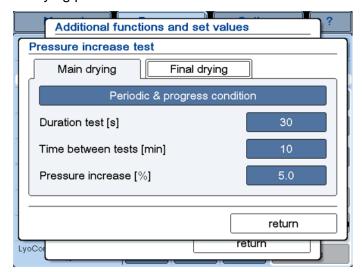


Fig. 65: Dialog box "Pressure increase test" in the program mode



Option: → Comparative pressure measurement (see chapter 6.7 - "Optional extensions and special equipment")



The indication of the measurement value "dp Comp" can be configured in chapter 6.6.1.1 - "Main window "Manual"" under "Actual values of the current process" in the dialog box "Select actual value".



If only capacitive sensors are permissible (e.g. for freeze-drying solvent-containing products), comparative pressure measurement is not possible.

The comparative pressure measurement can be activated or deactivated by pressing the button in the dialog box.

#### Progress condition:

If the difference between the readings of the Pirani and the capacitive vacuum sensor at the end of the last main drying section is below the limit " $\triangle$ p Comparative", the drying process will be considered complete at the current shelf temperature and chamber vacuum. Thus, the progress condition for switching to the next section is fulfilled and the next section will be initiated.

If the condition for switching to the next section is not fulfilled, a process message will be issued, the current section will be extended, and further pressure increase tests will be executed periodically until the condition is fulfilled.

#### Disabled:

There will be no comparative pressure measurement during the main drying phase. There will be no evaluation.

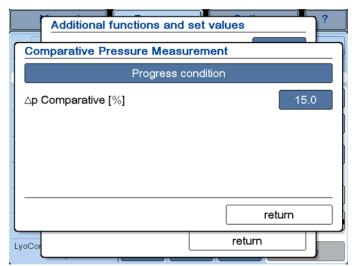


Fig. 66: Dialog box "Comparative pressure measurement"

#### 6 Operation




Option: LyoBalance weighing system

If the freeze-dryer is equipped with a LyoBalance weighing system (see chapter 6.7 - "Optional extensions and special equipment"), then the corresponding parameters must be configured in this dialog box.



Please refer to the separate operating manual of the weighing system!

Special equipment: → Aeration, stoppering, storage (see chapter 6.7 - "Optional extensions and special equipment")

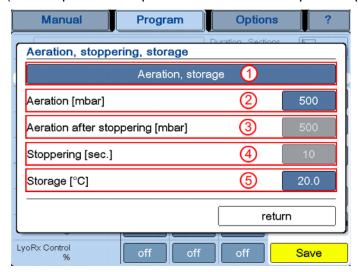

- 1 Button for selecting the variant
- 2 Set value "Aeration"
- 3 Set value "Aeration after stoppering"
- 4 Set value "Stoppering"
  - Set value "Storage"

Fig. 67: Dialog box "Aeration, stoppering, storage"

Repeated pressing of this button enables the user to choose between the following variants:

- Deactivated
- Aeration (up to the "Aeration" value) and subsequent storage
- Stoppering (at drying vacuum followed by aeration up to atmospheric pressure) with subsequent storage
- Aeration (up to the "Aeration" value), stoppering (followed by aeration up to atmospheric pressure) with subsequent storage

The set values of the parameters can be adapted by way of the respective button if the button is shown with a blue background.



A set value for the aeration ≤ 10 mbar can only be reached if the freezedryer is equipped with a precision needle valve for the gas injection.



"Aeration, (stoppering), storage" procedure:

1. Aeration up to the desired partial vacuum ("Aeration" value):
After the actual freeze-drying process has been completed, the ice
condenser continues to be cooled and the shelves are held at the
temperature of the last drying section. The system is aerated until the
desired partial vacuum is reached ("Aeration" value, see the illustration
above, item 2).



The product vials must be sealed at a chamber pressure below 900 mbar in order to prevent the stoppers from being pushed out of the vials at low atmospheric pressure.



If the set value for the aeration is below the current chamber pressure, the aeration phase will be skipped. The current chamber pressure will be maintained.

- 2. Stoppering followed by aeration up to atmospheric pressure While the ice condenser continues to be cooled and the shelf temperature is maintained, the shelves are moved together in order press the Lyo stoppers into the product vials. The stoppering pressure is maintained over the specific "Stoppering" time (see the illustration above, item 4). The subsequent final aeration is performed in two steps. In the first step, the system is aerated up to the partial vacuum that is stated under "Aeration after stoppering" (see the illustration above, item 3). Then, the shelves are moved apart into the drying position. In the second step, the system is aerated up to atmospheric pressure. This method prevents the stoppers from being ejected from the vials (if the shelves are moved apart without any prior aeration) and also from sticking to the shelves (if the shelves are not moved apart until the aeration to atmospheric pressure is complete).
- 3. Storage under defined conditions The shelves are brought to the set "Storage" temperature (see the illustration above, item 5) in order to store the product under optimum conditions. These conditions are kept constant until the system is manually set to the standby mode for unloading.



If the variant "Aeration, storage" has been selected, the product is stored at the "Aeration" pressure. In this case, the system must be aerated manually up to atmospheric pressure prior to opening the loading door.

Parameter	No.	Value range	Default setting
Aeration	2	0.001 mbar900 mbar	500 mbar
Aeration after stoppering	3	0.001 mbar900 mbar	500 mbar
Stoppering	4	1 sec999 sec	10
Storage	5	-99.9°C60.0°C	20°C



Special equipment: Preselection of the aeration medium

If the freeze-dryer is equipped with an automatic aeration valve and automatic valves for media selection, this dialog box can be used to preselect the medium that is to be used for the aeration medium requests during the execution of the particular program.

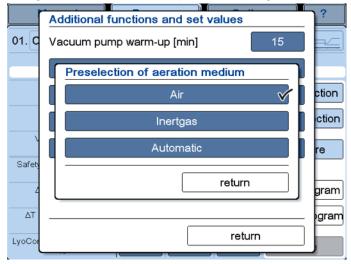


Fig. 68: Dialog box "Preselection of aeration medium"

If the vacuum control system of the freeze-dryer uses a regulated gas admission (injection), the preselected medium will be used for this purpose. If the freeze-dryer is equipped with the "Aeration, Stoppering, Storage" option, the preselected medium will be used for the aeration up to stoppering (backfilling) as well as for the final aeration up to atmospheric pressure.

The following media preselection settings are possible:

- Air: Preselects the media connection "Air".
- Inert gas: Preselects the media connection "Inert Gas".
- Automatic: Automatic media connection preselection depending on the chamber pressure and stoppering status of the product vials:
  - Chamber pressure ≥ 950 mbar or product vials already sealed by way of "Aeration, Stoppering, Storage": Preselection of the media connection "Air".
  - Chamber pressure < 950 mbar and product vials not yet sealed by way of "Aeration, Stoppering, Storage": Preselection of the media connection "Inert gas".

As a result, during automatic aeration, stoppering, and storage, backfilling can be performed automatically with inert gas and the subsequent aeration of the chamber up to atmospheric pressure with air.

Special equipment: Gas injection with a proportional valve (4)
See chapter 6.6.1.3 - "Main window "Options"", section "Special equipment:
Gas injection with a proportional valve"



#### **Program templates (2)**

The PGMplus programmer module offers various program templates that include recipes for all kinds of freeze-drying applications. They are suggestions for orientation purposes and must be adapted to the specific area of application of the freeze-dryer.



Some of the tests that are described under chapter 6.6.1.1 - "Main window "Manual"", section "Operating mode: select/start", are also available in the form of program templates.

Following the selection of a program template, a window containing information concerning the drying process will be displayed.

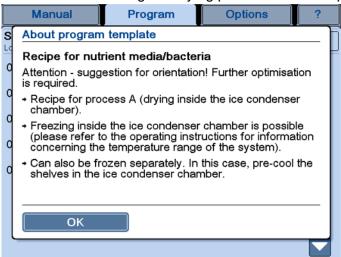


Fig. 69: Information concerning the program template (here: a recipe for nutrient media/bacteria)

After the conformation of the information, the program template will be displayed.

• Similar to a blank program, sections can be added or deleted and the set values can be adapted accordingly.

#### 6.6.3.2 Editing a program

An existing program can be modified as long as it has not been loaded.

- Select the program to be edited from the list in the main window "Program".
- Press the button with the program name in order to call up a window that displays the program data.
- Perform the desired modifications and save the program (see chapter 6.6.3.1 - "Creating a program").
- Close the dialog box by pressing the "Program" button.

The program has now been changed in the existing program storage location.



It is possible to switch to the manual mode during a program run, e.g. in order to edit a program during the runtime. The point of time for continuing the program run can be defined by selecting the desired start section and a start time.



#### 6.6.3.3 Copying a program

If a new program is to be created based on an already existing program, the already existing program can be copied. A free program storage location must be available for this purpose.

- Select the program to be copied from the list in the main window "Program".
- Press the button with the program name in order to call up a window with the program data.
- Press the button "Copy program" in order to create a copy of the existing program.
- Edit and save the copy (see chapter 6.6.3.1 "Creating a program").
- Close the dialog box by pressing the "Program" button.

The program will be automatically assigned to the first free program storage location.

#### 6.6.3.4 Loading a program

If a freeze-drying process is to be executed and controlled by a program, the program must be loaded.

- Call up the main window "Program". This window includes a list of all the programs that are saved.
- Press the button "Load" behind the program name. A dialog box will be displayed in which the start section, the start time or the start temperature can be adapted to any specific needs. The "Info" button can be used to call up a brief description of the active program, including information concerning the remaining runtime and the end of the program. It also enables a graphical representation of the process sequence.

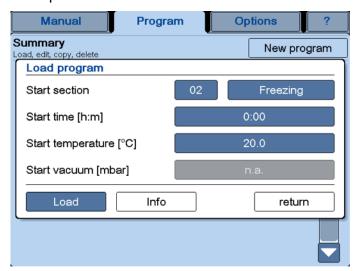


Fig. 70: Dialog box "Load program"

- Press the button "Load" in order to accept the program data. The display switches to the standard user interface.
- Press the button "Program start" in order to start the freeze-drying process.





Fig. 71: The freeze-drying process can be started with the aid of the button "Program start".

- During the freeze-drying process, the description of the active program can also be called up from the main window "Program" and via the button "Info".
- When the "Stop" button is pressed, the freeze-dryer switches to the standby – manual freezing mode.



The program starts with section 02 "Freezing" by default. If, however, section 01 "Load" is to be used as the starting point of the program, this section must be selected manually. In this case, the button "Program continue" will be displayed after the start of the program. When the precooling (loading) process is complete, this button must be pressed in order to continue with the program.

#### 6.6.3.5 Deleting a program

The PGMplus programmer module offers 32 program storage locations. If they are all occupied, a program must be deleted before a new one can be created.

- Select the program to be deleted from the list in the main window "Program".
- Press the button with the program name in order to call up a window with the program data.
- Press the button "Delete program". The system will then display a dialog box with an enquiry.
- Following the confirmation of the enquiry, the program will be deleted.

The program storage location on the list is now empty and the number is not shown on the list.



## 6.7 Optional extensions and special equipment

The freeze-dryer can be equipped with the following optional equipment. Special equipment cannot be retrofitted.

#### Option: Controlled Nucleation LyoCoN

The LyoCoN process enables the simultaneous freezing of all vials inside the drying chamber. To this end, ice crystals are accumulated on the cold ice condenser. At the same time, the liquid product is cooled to a temperature close to the freezing point. Then, a slight vacuum is generated inside the freeze-dryer. A reservoir, which has been installed externally, remains at atmospheric pressure. When the valve between the external reservoir and the ice condenser chamber is opened, the pressure will be equalised. The gas that passes by the ice condenser produces an extremely fine ice mist inside the drying chamber. This ice mist enters into all of the vials, thereby causing immediate and homogeneous freezing.

## Option: Wireless product temperature measurement system WTMplus

The wireless product temperature measurement system WTMplus has been developed mainly for freeze-dryers in the production area. The sensors are positioned directly in the product. They transfer their measurement values to an antenna that is integrated in the drying chamber. This enables the continuous monitoring of all of the phases of the freeze-drying process.

#### **Option: Pressure increase test**

see also chapter 6.6.3.1 - "Creating a program", button ">>more"

The pressure increase test can only be performed with the  $\rightarrow$  double-chamber method. During the pressure increase test, the intermediate valve prevents the flow of steam from the drying chamber to the ice condenser so that the water vapour of the  $\rightarrow$  sublimation cannot flow off. The result is a more or less distinct pressure increase that is measured in the product chamber. The pressure increase test is used as a criterion for the automatic switching from the main drying phase to the final drying phase as well as for identifying the end of the process.

## **Option: Improved cooling rate (fast freezing)**

Refrigeration unit 1 is used for cooling the ice condenser. Refrigeration unit 2 cools the heat transfer fluid that is used for controlling the temperature of the shelves. If the device option "Improved cooling rate" is activated (see chapter 6.6.1.3 - "Main window

"Options""/Administration/Device options), the ice condenser refrigeration unit will be used during the "Freezing" phase to support the cooling of the heat transfer fluid. This enables higher freezing rates

This option is only available for freeze-dryers of the Epsilon 2-6D LSCplus and Epsilon 2-10D LSCplus type.



#### Option: LyoCam monitoring camera system

The LyoCam monitoring camera system is used to monitor and analyse freeze-drying processes. A high-quality camera takes pictures of the product at intervals from several seconds to several minutes. The intervals are variable depending on the process section. The pictures are linked to the LPCplus SCADA system for process visualisation and they are assigned a time stamp in line with other recorded process parameters.

#### **Option: Comparative pressure measurement**

see also chapter 6.6.3.1 - "Creating a program", button ">>more"

During the  $\rightarrow$  *sublimation*, i.e. when the concentration of water vapour molecules is rather high in the atmosphere, the value that is provided by the gas-type-dependent vacuum sensor of the "Pirani" type (e.g. Thyracont VCP 63) in the drying chamber deviates from the value that is provided by a capacitive vacuum sensor (e.g. MKS 722B). When the proportion of water vapour molecules decreases towards the end of the main drying phase, the two sensors fall increasingly in line with one another. This difference will be evaluated and used as an indicator for identifying the drying end of the main drying phase.

#### **Option: LAN process recording (RJ45)**

This feature enables the recording of a running process directly on a PC/laptop computer. During the process recording, the process data can be viewed on the PC with LyoLogplus and they can be printed. It is also possible to import the data directly into an Excel file after the completion of the process recording.

#### Option: LyoControl measuring system

The Lyo Control measuring system can be used to determine the crystallisation state of the product. In the liquid state, the electrical resistance is very low. During the freezing process, the resistance increases. The LyoRx control sensor measures the electrical resistance.

### Option: LyoLogplus data logging software

LyoLogplus is a data logging software program by Martin Christ Gefriertrocknungsanlagen GmbH that is specifically adapted to the requirements of freeze-drying processes. Apart from the graphical representation of the measurement data of currently running processes, it also enables the data export for additional evaluation.

## **Option: LPCplus SCADA System**

The Christ LPCplus system consists of the <u>Supervisory Control And Data Acquisition</u> (SCADA) software program by Martin Christ Gefriertrocknungsanlagen GmbH and a dedicated PC. The system is connected to the LSCplus controller of the freeze-dryer via Ethernet and provides the operation of all of the freeze-drying functions as well as process recording (measurement data and process events), process documentation and data backup. Furthermore, it enables the comfortable administration of freeze-drying programs/recipes and users.



#### **Option: USB process recording**

see also chapter 6.6.1.1 - "Main window "Manual"", section "Dialog box "Tools""

This feature enables the recording of a running process on a USB storage medium. After the end of the process recording, the process data can be viewed on the PC with LyoLogplus and they can be printed. It is also possible to import the data directly into an Excel file.

#### Option: LyoBalance weighing system

see also chapter 6.6.1.1 - "Main window "Manual"", section "Dialog box "Tools""

The LyoBalance weighing system enables the user to determine the weight loss of a product during a freeze-drying process. The drying rate that results from the weight loss provides information concerning the progress of the freeze-drying process. Thereby, it also helps the user to determine the end of the freeze-drying process and to optimise the process parameters.

#### Special equipment: Aeration, stoppering, storage

see also chapter 6.6.3.1 - "Creating a program", button ">>more"

This option is available only in combination with the PGMplus programmer module and if the freeze-dryer is equipped with an automatic aeration valve and a hydraulic shelf movement system. It offers automatic sealing of the product vials with pre-inserted rubber stoppers under partial vacuum and subsequent storage on the shelves under defined conditions as an integral part of a freeze-drying program.

## Special equipment: Gas injection with a proportional valve

see also chapter 6.6.1.3 - "Main window "Options"", section "General" If the freeze-dryer is equipped with a proportional gas injection valve, the method that is to be used for vacuum control can be preselected. The method can be saved together with a recipe.

#### **Special equipment: Inertisation**

see also chapter 6.6.1.3 - "Main window "Options"", section "General" If products containing solvent are dried in an oxygen atmosphere, explosive mixtures may form. In order to dry these types of products, the freeze-dryer must be equipped with a door-controlled inertisation system that uses nitrogen or another inert gas.

#### Special equipment: Preselection of the aeration medium

see also chapter 6.6.1.3 - "Main window "Options"", section "General"

If the freeze-dryer is equipped with an automatic aeration valve and automatic valves for media selection, a special medium can be preselected that is to be used for all of the aeration medium requests as of the start of the main drying phase.



# 6.8 Switching the freeze-dryer OFF

The freeze-dryer must be in the standby status.

• Switch the freeze-dryer off by pressing the mains switch.



## 7 Malfunctions and error correction

Malfunctions are displayed in the dialogue box "Process & equipment messages" (see chapter 7.2 - "Process and error messages"). An acoustic signal sounds when an error message is generated.

- Eliminate the source of the problem (see the following chapter).
- Acknowledge the error message.

## 7.1 General malfunctions

Type of error	Possible reason	Correction
No indication on the display	<ul> <li>No power in the mains supply (see chapter 7.1.1 - "Power failure").</li> <li>Power cord is not plugged in.</li> <li>Fuses have tripped.</li> <li>The mains power switch is set to off.</li> </ul>	<ul> <li>Check the mains power supply fuse.</li> <li>Plug in the power cord correctly.</li> <li>Check the on-site fuses</li> <li>Switch mains power switch ON.</li> </ul>
The touchpanel does not react at all or it does not react correctly	The sensitivity of the touchpanel is misadjusted.	Contact the service department (see chapter 7.3 - "Service contact")
The password input fails	The password is not correct.	<ul> <li>Inform the administrator.</li> <li>If you have lost the administrator password: contact the service department (see chapter 7.3 - "Service contact")</li> </ul>
Insufficient vacuum	Incorrect connection of the small flange connection(s).	<ul> <li>Loosen the connection. Place the centring ring with the inner sealing ring in a centred manner between the flange connections and connect it with the clamping ring. Ensure that the centring ring neither slips out of place nor gets jammed.</li> </ul>
	Dirty or damaged lid or door seal.	<ul> <li>Clean the lid or door seal and replace it if necessary.</li> </ul>
	<ul> <li>The ground-in stopper of the attached drying chamber is not installed correctly.</li> </ul>	<ul> <li>Grease the ground-in stopper evenly and over the entire sealing surface with vacuum grease.</li> </ul>
Leakage in the media drain valve	<ul> <li>The media drain valve is soiled with drying residues or wool particles from cleaning cloths.</li> <li>The O-rings are worn</li> </ul>	<ul> <li>Clean the media drain valve (see chapter 8.1.3 - "Aeration valve") and replace it if necessary.</li> <li>Replace the O-rings.</li> </ul>
Leakage in a rubber valve	The valve is soiled.	Check the valves individually (see chapter 7.1.2.4 - "Rubber valves")



#### 7 Malfunctions and error correction

Type of error	Possible reason	Correction
The displayed vacuum value is not correct	Incorrect calibration	<ul> <li>Calibrate the vacuum sensor (see the separate operating instructions of the vacuum sensor).</li> </ul>
	The vacuum sensor is soiled (e.g. due to water residues)	Clean the vacuum sensor.
	<ul> <li>The vacuum sensor is defective.</li> </ul>	<ul> <li>Check the vacuum display with the aid of a reference device (if available).</li> <li>see chapter 7.1.2.5 - "Vacuum sensor"</li> </ul>
		sensor
The vacuum pump is not activated	<ul> <li>See the separate operating instructions of the vacuum pump.</li> </ul>	<ul> <li>See the separate operating instructions of the vacuum pump.</li> </ul>
Insufficient ice condenser or shelf temperature	The overpressure switch of the refrigeration unit has tripped.	Let the unit cool down.
	The thermal circuit breaker has tripped.	Ensure sufficient air circulation (see chapter 7.1.3 - "Insufficient ice condenser temperature")
The error message "Refrigeration unit x.x overpressure" is displayed during a freeze-drying process	Leakage on the low pressure side (suction side) of the refrigeration system leads to a pressure increase	Acknowledge the message.  If the message is displayed repeatedly, inform the service department (see chapter 7.3 - "Service contact")



If it is impossible to eliminate the errors, contact the Christ service department!

#### 7.1.1 Power failure

The control system continues with the process after a power failure. The preselected conditions remain saved even during a process run. In the event of a power failure in the drying phase, the batch may become unusable. Whether the batch can be saved or not depends on the drying phase in which the product was when the power failure occurred.

- In the final drying phase, the product has reached a residual moisture content of approx. 5%. Below this value, the product is generally not damaged even if the power failure lasts for a longer period of time.
- If the product is in the main drying phase, we recommend aerating the unit, removing the product, and storing it in a deep-freeze. The defrosted condensate must be drained off prior to the next start.



#### 7.1.2 Insufficient vacuum



The vacuum checks must be carried out when the ice condenser is frozen.

#### 7.1.2.1 Small flange connections

Leakages are often due to improper small flange connections between the various components and hose connections or to leakages in the valves.

- Loosen the connection and place the centring ring (with sealing ring inside) in a centred manner between the flange connections.
- Seal the connection with the clamping ring by tightening the wing nut.
- Ensure that the centring ring neither slips out of place nor gets jammed.



Fig. 72: Small flange and centring ring



Fig. 74: Attaching the clamping ring



Fig. 73: Small flange with centring ring and small flange



Fig. 75: Tightened clamping ring



#### 7.1.2.2 Aeration valve

A malfunction of the aeration valve may have several causes. One potential source are contaminants such as product residues within the valve.

- Switch the freeze-dryer off and disconnect the mains plug.
- Clean the valve (see chapter 8.1.3 "Aeration valve").
- Put the freeze-dryer into operation again.

If there is still a leakage, the freeze-dryer must be checked by qualified specialist personnel (see chapter 7.3 - "Service contact").

#### 7.1.2.3 Pressure control valve

A malfunction of the pressure control valve may have several causes.



The inspection of the valve must be carried out by qualified specialist personnel (see chapter 7.3 - "Service contact").

#### 7.1.2.4 Rubber valves

In order to identify a leaking rubber valve, the valves must be checked individually:

- Remove the rubber valve and seal the connection at the drying chamber with a rubber stopper.
- Check the tightness under vacuum until the leaking valve has been localised.
- Clean the valve or replace it if necessary.

#### 7.1.2.5 Vacuum sensor

Vacuum sensors have a limited service life and can be ordered as spare parts.

#### Capacitive vacuum sensors

Capacitive vacuum sensors may experience a measurement drift due to long-term use, soiling or sudden aeration. In this case, the vacuum sensor must be adjusted (see chapter 8.1.9 - " Vacuum sensor ").



#### 7.1.3 Insufficient ice condenser temperature



Ensure sufficient ventilation. Do not place any paper, cloth, or similar material behind or under the unit, since otherwise the air circulation will be impaired.

The refrigeration unit is equipped with a protective device against overpressure in the refrigeration system and with a thermal motor protection switch.

The protective devices trip

- when the ambient temperature is too high
- when the air circulation of the heat exchanger of the refrigeration system is insufficient
- when the refrigeration system is overloaded.

In these cases, the refrigeration unit will be switched off automatically. If the permissible operating conditions are re-established after a cool-down phase of several minutes, the refrigeration unit will be switched on again automatically.

The malfunctions are displayed in the process and equipment information window.

The minimum ice condenser temperature of approx. -55°C or approx. -85°C (depending on the type of freeze-dryer) is reached when the ice condenser is not loaded and the ice condenser chamber is evacuated.

# 7.2 Process and error messages

The control system displays the complete process and error messages (see chapter 6.6.1.1 - "Main window "Manual"", dialogue box "Process and equipment messages"), which is why they are not included in this operating manual.

You can order these documents from our service department.



#### 7.3 Service contact

In the event of queries, malfunctions, or spare part enquiries:

#### From Germany:

Contact

Martin Christ Gefriertrocknungsanlagen GmbH An der Unteren Söse 50 37520 Osterode (Germany) Tel. +49 (0) 55 22 / 50 07-33 33

E-mail: support.epsilon@martinchrist.de

#### **Outside Germany:**

Contact our agency in your country. All agencies are listed at  $\underline{www.martinchrist.de} \rightarrow [Sales Partners]$ 



If you would like to utilise our after-sales-service, please state the type
of your freeze-dryer and its serial number.



The freeze-dryer and the accessories are subject to high mechanical and chemical stress. Thorough maintenance performed by the user extends the service life and prevents premature failure.



If corrosion or other damage occurs due to improper care, the manufacturer cannot be held liable or subject to any warranty claims.

- Thoroughly clean the freeze-dryer immediately after use to prevent or at least significantly reduce the damage to the materials of construction (see also chapter 1.3.1 - "Freeze-drying of solvent-containing products (non-aqueous media)").
- Use soap water or other water-soluble, mild cleaning agents for cleaning the freeze-dryer and the accessories.
- Do not use corrosive and aggressive substances.
- · Do not use solvents.
- · Do not use agents with abrasive particles.
- Do not expose the freeze-dryer or its accessories to intensive UV radiation (e.g. sunlight) or thermal stress (e.g. by heat generators).
- Do not turn the unit upside down in order to clean it.

#### 8.1 Maintenance

#### 8.1.1 General

The general state of the freeze-dryer must be checked at regular intervals. Any defects must be eliminated immediately! The following points are of particular importance:

- dirt,
- leaks,
- corrosion.
- bent system components,
- · loose screw and flange connections,
- · higher noise levels,
- loose cables,
- open cable ducts,
- missing or illegible safety notes and hazard warnings,
- missing or illegible inscriptions on components, pipes (direction of flow) and cables,
- · etc.



#### Cleaning of the freeze-dryer



#### Risk of burns on hot surfaces

#### Housing of the freeze-dryer

During the operation of the freeze-dryer and half an hour afterwards, the outer surface of the freeze-dryer (especially the pipes and units) may be hot.

#### Inside the chamber:

After a drying process, some or all of the surfaces inside the chamber (chamber walls, shelves, intermediate valve, etc.) may still be hot.

There is a risk of burns when touching the surfaces.

- · Wear suitable protective clothes and gloves!
- Do not touch the surfaces on purpose!



#### Risk of poisoning/infection caused by the products

When performing maintenance work on parts coming into contact with the product (e.g. all parts inside the chamber, vacuum pump), the personnel may be exposed to product residues.

Skin contact or the inhalation of particles may cause severe damage to health depending on the product in question.

- Take suitable decontamination measures prior to commencing the maintenance!
- Wear suitable protective clothes and gloves!
- Switch the freeze-dryer off by actuating the mains power switch and disconnect the power cord from the wall outlet before cleaning.
- If the freeze-dryer has been contaminated with toxic, radioactive, or pathogenic substances, clean the inside immediately with a suitable decontamination agent (depending on the type of contamination, see chapter 8.2 "Disinfection of the drying chamber and accessories").
- Remove product residues thoroughly with a cloth.
- Open loading door when the freeze-dryer is not in use so moisture can evaporate.

#### 8.1.2 Chamber

In order to avoid corrosion and negative effects on a subsequent freezedryer process, it must be ensured that there is no water left inside the drying chamber after every freeze-drying process.

- Empty the defrosting water collecting tray and wipe it dry.
- If necessary, wipe the ice chamber dry with a cloth.



#### 8.1.2.1 Lamination of the loading door with a special film

Freeze-dryers with an acrylic glass door are equipped with the special Radiation Shield film on the exterior side of the acrylic glass door (see chapter 6.5 - "Loading door").



For technical reasons, inclusions are possible. However, they do not prevent the film from performing its function.



In the case of acrylic glass doors with a Radiation Shield film, visible light reflexions are possible. This is not a defect but rather the natural consequence of the high-performance film.

To prevent the film from being damaged, compliance with the following points is mandatory for cleaning:

- In case of a contamination with toxic, radioactive or pathogenic substances, clean immediately with a suitable decontamination agent (see chapter 8.2 - "Disinfection of the drying chamber and accessories").
- Clean with plenty of water immediately after use to ensure that contaminants are flushed off and not wiped off.



Do not clean the film while dry.


- Use soft cloths, soft sponges made of synthetic fibres or rubber squeegees and common household cleaning agents (glass cleaner) for cleaning. The cleaning agents must be free from abrasive agents.
- Do not use hard sponges, cloths or brushes for cleaning.
- Avoid strong mechanical stress during cleaning.



#### 8.1.2.2 Door latch

There is a slide pad on the door latch of the loading door. This slide pad is included in the scope of supply as a spare part (part no. 18189991). It must be inspected regularly for signs of wear. When its thickness is < 0.5 mm, it must be replaced.

- 1 Door latch
- 2 Slide pad
- 3 Torx screws






Fig. 76: Door latch and slide pad


#### Replacing the slide pad:

Unscrew the two screws of the slide pad with a Torx® TX10 screwdriver, remove the old slide pad, and install the new one.

#### 8.1.3 Aeration valve

Contaminants such as product residues may lead to an insufficient vacuum. In this case, the aeration valve must be cleaned.

- Switch the freeze-dryer off and disconnect the mains plug.
- Remove the valve core.
- Clean the valve core and the opening with a moist cloth.
- Clean the O-rings and inspect them for any damage. Damaged O-rings must be replaced.



- 2 Valve core
- 3 O-rings

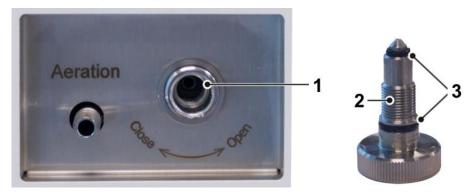


Fig. 77: Valve opening and valve core with O-rings (example)

- If necessary, grease the valve core with a thin layer of high-vacuum grease and (part no. 126210) reinsert the valve core.
- Put the freeze-dryer into operation again.

If the vacuum is still insufficient, the freeze-dryer must be checked by qualified specialist personnel (see chapter 7.3 - "Service contact").



#### 8.1.4 Heat exchanger (only air-cooled freeze-dryers)

A lamellar heat exchanger is used for cooling the refrigerant that is compressed by the refrigeration unit. This air-cooled heat exchanger is located at the back of the unit (see chapter 2.1.1 - "Functional and operating elements").

Dust and dirt impair the cooling effect of the air flow. Dust on the lamellas prevents the exchange of heat and, thereby, impairs the performance and power of the refrigeration unit. Strong soiling may cause the unit to fail.

This is why the selected set-up location should be as clean as possible.

- Check the heat exchanger at least once per month for soiling and clean it if necessary.
- Please contact the Christ service department if you have any queries (see chapter 7.3 "Service contact").

#### 8.1.5 Electrical system



#### Danger of life caused by electric shock

There is a risk of electric shock when touching current-carrying components.

This may lead to ventricular fibrillation, cardiac arrest, or respiratory paralysis.

 Only qualified electricians are authorised to perform work on the electrical system of the freeze-dryer!

The electrical equipment of the freeze-dryer must be checked at regular intervals by a qualified electrician. Defects such as loose connections or burnt cables must be eliminated immediately.



#### 8.1.6 Vacuum system with an oil-sealed vacuum pump



Please refer to the maintenance instructions of the vacuum pump and exhaust gas filter in the enclosed operating instructions of the manufacturer!



#### Risk of burns on hot surfaces

During the operation of the freeze-dryer and half an hour afterwards, the outer surface of the vacuum pump may be hot.

There is a risk of burns when touching the surfaces.

- Prior to performing any maintenance work on the vacuum pump or the oil mist separator, let the components cool!
- Wear suitable protective clothes and gloves!



#### Risk of scalding caused by the vacuum pump oil

When working on the vacuum pump and exhaust gas filter (especially when changing the oil or filter), the maintenance personnel are exposed to the hot vacuum pump oil.

There is a risk of scalding in the event of skin contact.

- · Wear suitable protective clothes and gloves!
- · Use a suitable collecting vessel!



#### Risk of poisoning/infection caused by the vacuum pump oil

When working on the vacuum pump and exhaust gas filter (especially when changing the oil or filter), the maintenance personnel are exposed to the vacuum pump oil, which may contain harmful substances originating from the product. In addition, synthetic oils can release toxic fumes when they are ignited or heated above 300°C.

The inhalation of the fums that are released by the oil, or contact with the skin, can cause severe damage to health.

- Wear suitable protective clothes, gloves, and respiratory protection!
- Ensure the environmentally sound disposal of the oil in compliance with the local rules and regulations!
- Do not let the oil come into contact with tobacco products!

The stress of the vacuum pump in conjunction with a freeze-dryer is usually not very high. This is why the recommendations in this operating manual may differ from the information that is provided by the pump manufacturers.

Under normal operating conditions, the following maintenance tasks concerning the vacuum pump must be performed at regular intervals:

- Check the oil level of the vacuum pump once per week. If necessary, top it up with oil.
- Check the running pump for any unusual noise.
- Ensure that the pump has reached its operating temperature prior to changing the oil. If the oil is cloudy, shows particles or is discoloured, an oil change must be performed.
- Perform the first oil change after approximately 100 operating hours.





- The other oil changes depend on the operating conditions. In general, an interval of 500 to 1,000 operating hours is sufficient.
- Please contact the Christ service department if you have any queries (see chapter 7.3 "Service contact").

#### 8.1.7 Vacuum system with a dry-running vacuum pump

The dry-running vacuum pump requires only minimal maintenance.



Comply with the maintenance instructions of the manufacturer in the separate operating instructions of the vacuum pump and silencer!

In addition, the following must be taken into consideration:



#### Risk of burns on hot surfaces

During the operation of the freeze-dryer and half an hour afterwards, the outer surface of the vacuum pump may be hot.

There is a risk of burns when touching the surfaces.

- Prior to performing any maintenance work on the vacuum pump, let the components cool!
- Wear suitable protective clothes and gloves!



#### Danger of poisoning/infection due to contaminated exhaust air

The exhaust air may contain harmful substances originating from the product.

Contact with particles in the exhaust air (especially by inhalation) may result in severe damage to health.

- Use a silencer with integrated filter elements or depending on the product – guide the exhaust gases from the outlet of the vacuum pump to a suitable treatment system in order to prevent the discharge of harmful substances into the surrounding atmosphere! Compliance with the national rules and regulations for the protection of the environment must be ensured!
- When working on the vacuum system (and especially on the vacuum pump), it may be necessary to wear suitable protective clothing, gloves and a breathing mask depending on the product!

The number of operating hours of the vacuum pump can be monitored by way of the LSCplus control system and also by way of the CHRIST SCADA software LPCplus (see chapter 6.6.1.3 - "Main window "Options""/"Operating hours" and "Vacuum pump oil change" or separate operating manual of the Christ SCADA software LPCplus, index entries "Working hours" and "Oil change interval (vacuum pump)").



#### 8.1.8 Refrigeration system



#### Risk of suffocation caused by the refrigerant

When work is performed on the refrigeration system of the freeze-dryer, refrigerant may escape in the liquid or gas state and under high pressure. Gaseous refrigerant is heavier than air and high concentration levels of it may collect on the floor or in pits.

There is a risk of suffocation in the case of high concentration levels. Possible symptoms are paralysis and unconsciousness. Affected persons do not notice the fact that they suffocate.

- Only qualified persons are authorised to perform work on the refrigeration system of the freeze-dryer!
- Ensure good aeration/extraction when working on the refrigeration system!



#### Risk of cold burns or frostbite caused by the refrigerant

When work is performed on the refrigeration system of the freeze-dryer, refrigerant may escape in the liquid or gas state and under high pressure. In the case of skin contact with liquid refrigerant, cold burns or frostbite may result.

 Only qualified persons are authorised to perform work on the refrigeration system of the freeze-dryer!



#### Risk of explosion due to refrigerants

The natural refrigerants used are highly flammable and can form an explosive mixture if their concentration in the ambient air is sufficiently high.

There is an explosion hazard.

- Work on the refrigeration system of the freeze-dryer must only be carried out by qualified specialist personnel who have been trained to handle flammable refrigerants!
- Ensure good ventilation and make sure that no ignition sources (e.g. soldering iron, welding equipment) are present!

The refrigerant circuit is a closed system. Only certified and qualified persons are authorised to perform work on the refrigeration system!



#### 8.1.9 Vacuum sensor



Please refer to the separate operating manual of the vacuum sensor!

The vacuum sensor has only a limited service life.

- The vacuum sensor is maintenance-free.
- Remove any soiling on the outside with a cloth.

#### Option: capacitive vacuum sensors

Measurement drift due to long-term use, soiling or sudden aeration may occur.

Capacitive vacuum sensors must be adjusted at least once per year.
 Depending on the actual conditions of use, shorter adjustment intervals may be necessary.

#### 8.1.10 Accessories



For the care of the accessories, special safety measures must be considered as these are measures that will ensure operational safety at the same time.

Chemical reactions as well as stress-corrosion (combination of oscillating pressure and chemical reaction) can affect or destroy the metal and plastic parts. Barely detectable cracks on the surface can expand and weaken the material without any visible signs.

- Check the material regularly (at least once a month) for
  - cracks
  - visible damage of the surface
  - pressure marks
  - signs of corrosion
  - other changes.
- Replace any damaged components immediately for your own safety.
- Immediately rinse off the accessories if any liquids that may cause corrosion come into contact with them.
- Clean the accessories outside the freeze-dryer once a week or preferably after each use.



# 8.2 Disinfection of the drying chamber and accessories



If dangerous materials (e.g. infectious and pathogenic substances) are used, the freeze-dryer and accessories must be disinfected.

- Use commercially-available disinfectants such as, for example, Incidur®, Meliseptol®, Sagrotan®, Buraton®, or Terralin® (available at specialised trade).
- The freeze-dryers and the accessories consist of various materials. A
  possible incompatibility must be considered.
- Before using cleaning or decontamination agents that were not recommended by us, contact the manufacturer to ensure that such a procedure will not damage the freeze-dryer.
- Please contact us if you have any queries (see chapter 7.3 "Service contact").



# 8.3 Maintenance schedule (oil-sealed vacuum pump)

for freeze-dryers with an oil-sealed vacuum pump



# Tests and checks in accordance with the statutory rules and regulations

Compliance with the applicable national and international laws, rules, and regulations concerning health and safety, the prevention of accidents, and the protection of the environment must be ensured.

Perform the prescribed regular tests and checks of the various components of the freeze-dryer (e.g. electrical equipment, safety devices, refrigeration systems) in accordance with the specifications!

System/ Component	Detail / Part	Inspe	ection	I	Periodical N	Maintenanc	e	Repair / Rebuild
		Before start	Per working day	Inspection	Replacement	Operation	Calibration	
Safety devices	See chapter 3.8 - "Safety devices"			Х		Х		
Drying chamber and loading door	Drying chamber: dry and clean	Х		х				
	Shelf surface: clean, undamaged	х		Х				
	Door gasket: clean, undamaged	х		Х	50 steril. cycles			Replacement procedure
	Door hinges			Х		Х		Adjustment after replacement of the door gasket
	Stainless steel door cover: securly attached	х		х				
	Stainless steel door sight glasses: clean, illumination ok	х		х				
	Acrylic glass door: surface clean and undamaged	х		х				
Machinery – general	Switch cabinet		Х	Х				
	Leakages		X	Х				
	Noise emission above average		Х	Х				
	Dynamic gaskets: diaphragmas				50 steril. cycles			



System/ Component	Detail / Part	Inspe	ection		Periodical N	/laintenanc	e	Repair / Rebuild
		Before start	Per working day	Inspection	Replacement	Operation	Calibration	
	Static gaskets: O-rings, clamp, KF				100 steril. cycles			
	Wires: fastened			Х				
	Cable trays: closed			Х				
	Framework: no corrosion			Х				Remove corrosion
Vacuum system	Pump: oil level	х	Х	Х				
	Pump: oil condition (colour, contamination)	Х	Х	X	oil change			
	Exhaust filter: emission of oil mist		х	X		X		
	Exhaust filter: oil level		х			X		Cleaning of the filter
	Residues / particles inside the housing			Х				
	Oil-leakage under the pump	Х		Х	after 10 years			Rotary shaft seal, bearings, vanes, springs: service life of 10 years
	Final vacuum					X		
	Vacuum leak test					Х		
Refrigeration system	Icing of components			Х				
	Pressure readings / performance tests					Х		
	Noise level above average			Х				
	Solenoid valves: operation					Х		
	Ice condenser: temperature low end			_		Х		



System/ Component	Detail / Part	Inspe	ection		Periodical N	Maintenanc	е	Repair / Rebuild
		Before start	Per working day	Inspection	Replacement	Operation	Calibration	
	Cooling water controller			Х		Х		Cleaning of the valve
	Heat exchanger			Х		Х		Cleaning
Vial stoppering system	Mechanical components: operation			X				
	Leakages		Х	X				
	Hydraulic system: maximum pressure reading					Х		
	Hydraulic system: oil in reservoir			Х				
	Hydraulic system: condition of the hoses			Х	after 5 years			Replace hose lines even if no safety- relevant defects can be noticed
	Hydraulic system: cylinder travel speed					Х		
Instrumentation	Vacuum sensor(s)						Х	Calibration
	Temperature sensors at freeze-dryer						Х	Calibration
	Pressure sensors chamber						Х	Calibration
	Product temperature sensors					Х	Х	Calibration, replacement of connectors
	Level switch(es)					Х		
	Pilot valves (Solenoid valves)			Х		Х		
Electrical installation	Switch cabinet: temperature inside			Х		Х		Infrared readings if possible
	Switch cabinet: condition of the components			Х				



System/ Component	Detail / Part	Inspection			Periodical I	Maintenanc	e	Repair / Rebuild
		Before start	Per working day	Inspection	Replacement	Operation	Calibration	
	Switch cabinet: cooling system			Х	1 year	Х		Replacement of the filter
	Wiring			Х				
	Power readings of components					Х		
	LSCplus control system			х	6 years	Х		Replacement of the buffer battery



## 8.4 Maintenance schedule (dry-running vacuum pump)

For freeze-dryers with a dry-running vacuum pump



# Tests and checks in accordance with the statutory rules and regulations

Compliance with the applicable national and international laws, rules, and regulations concerning health and safety, the prevention of accidents, and the protection of the environment must be ensured.

Perform the prescribed regular tests and checks of the various components of the freeze-dryer (e.g. electrical equipment, safety devices, refrigeration systems) in accordance with the specifications!

System/ Component	Detail / Part	Inspe	ection	l	Periodical N	Maintenanc	:e	Repair / Rebuild
		Before start	Per working day	Inspection	Replacement	Operation	Calibration	
Safety devices	See chapter 3.8 - "Safety devices"			Х		Х		
Drying chamber and loading door	Drying chamber: dry and clean	Х		Х				
	Shelf surface: clean, undamaged	х		Х				
	Door gasket: clean, undamaged	х		Х	50 steril. cycles			Replacement procedure
	Door hinges	х		Х		Х		Adjustment after replacement of the door gasket
	Stainless steel door cover: securly attached	х		х				
	Stainless steel door sight glasses: clean, illumination ok	х		х				
	Acrylic glass door: surface clean and undamaged	х		Х				
Machinery – general	Switch cabinet		Х	Х				
	Leakages		X	Х				
	Noise emission above average		Х	Х				
	Dynamic gaskets: diaphragmas				50 steril. cycles			



System/ Component	Detail / Part	Inspe	ection	-	Periodical I	Maintenanc	e	Repair / Rebuild
		Before start	Per working day	Inspection	Replacement	Operation	Calibration	
	Static gaskets: O-rings, clamp, KF				100 steril. cycles			
	Wires: fastened			Х				
	Cable trays: closed			Х				
	Framework: no corrosion			Х				Remove corrosion
Vacuum system	Pump: Inlet strainer			Х				Inspection and cleaning annually
	Pump: Gas ballast control			Х				Inspection and cleaning annually
	Pump: External fan cover			Х				Cleaning annually
	Pump: Tip Seals				9.000 operating hours			
	Pump: Condition of motor / drive			Х		Х		Inspection after every 15,000 operating hours
	Pump: Bearings				35.000 operating hours			
	Silencer: Filter element				9.000 Betriebs- std.			Exchange of the filter element
	Final vacuum					Х		
	Vacuum leak test					х		
Refrigeration system	Icing of components			Х				
	Pressure readings / performance tests					Х		
	Noise level above average			Х				
	Solenoid valves: operation					Х		



System/ Component	Detail / Part	Inspe	ection	ı	Periodical I	Maintenanc	е	Repair / Rebuild
		Before start	Per working day	Inspection	Replacement	Operation	Calibration	
	Ice condenser: temperature low end					Х		
	Cooling water controller			Х		Х		Cleaning of the valve
	Heat exchanger			Х		Х		Cleaning
Vial stoppering system	Mechanical components: operation			х				
	Leakages		Х	Х				
	Hydraulic system: maximum pressure reading					х		
	Hydraulic system: oil in reservoir			Х				
	Hydraulic system: condition of the hoses			X	After 5 years			Replace hose lines even if no safety- relevant defects can be noticed
	Hydraulic system: cylinder travel speed					X		
Instrumentation	Vacuum sensor(s)						Х	Calibration
	Temperature sensors at freeze-dryer						Х	Calibration
	Pressure sensors chamber						Х	Calibration
	Product temperature sensors					х	Х	Calibration, replacement of connectors
	Level switch(es)					Х		
	Pilot valves (Solenoid valves)			Х		Х		
Electrical installation	Switch cabinet: condition of the components			X				



System/ Component	Detail / Part	Inspection		l	Periodical N	:e	Repair / Rebuild	
		Before start	Per working day	Inspection	Replacement	Operation	Calibration	
	Switch cabinet: cooling system			Х	1 year	Х		Replacement of the filter
	Wiring			Х				
	Power readings of components					Х		
	LSCplus control system			Х	6 years	Х		Replacement of the buffer battery



#### 8.5 Service



In the event of service work that requires the removal of the panels, there is a risk of electric shock or mechanical injury. Only qualified specialist personnel is authorised to perform this service work.

The freeze-dryer is subject to high mechanical stress. In order to be able to withstand this high level of stress, high-quality components were used during the production of the freeze-dryer. Nevertheless, wear cannot be excluded and it may not be visible from the outside.

This is why we recommend having the freeze-dryer checked by the manufacturer during an inspection once per year.

# Information and appointments:

From Germany:

Contact

Martin Christ Gefriertrocknungsanlagen GmbH An der Unteren Söse 50 37520 Osterode (Germany) Tel. +49 (0) 55 22 / 50 07-33 33

E-mail: <a href="mailto:support.epsilon@martinchrist.de">support.epsilon@martinchrist.de</a>

#### **Outside Germany:**

Contact our agency in your country. All agencies are listed at www.martinchrist.de → [Sales Partners]



If you would like to utilise our after-sales-service, please state the type of your freeze-dryer and its serial number.

# 8.6 Return of defective parts

Although we exercise great care during the production of our products, it may be necessary to return a unit or accessory to the manufacturer.

In order to ensure the quick and economical processing of returns of freeze-dryers, rotational vacuum concentrators, spare parts, or accessories, we require complete and extensive information concerning the process. Please fill in the following forms completely, sign them, enclose them with the return package, and send them together with the product to:

Martin Christ Gefriertrocknungsanlagen GmbH An der Unteren Söse 50 37520 Osterode (Germany)



#### 1. Declaration of decontamination

As a certified company and due to the legal regulations for the protection of our employees and of the environment, we are obliged to certify the harmlessness of all incoming goods. For this purpose, we require a declaration of decontamination.

- The form must be filled in completely and signed by authorised specialist personnel only.
- Affix the original form in a clearly visible manner to the outside of the packaging.



We will return the part/unit if no declaration of decontamination is provided!

#### 2. Form for the return of defective parts

This form is for the product-related data. They facilitate the assignment, and they enable the quick processing of the return. If several parts are returned together in one packaging, please enclose a separate problem description for every defective part.

- A detailed problem description is necessary in order to perform the repair quickly and economically.
- Upon request, we will prepare and submit to you a cost estimate prior to performing the repair. Please confirm such cost estimate within 14 days. If the cost estimate has still not been confirmed after 4 weeks, we will return the defective part/unit. Please note that you must bear the incurred costs.



The part/unit must be packaged in a transport-safe manner. Please use the original packaging for the unit, if at all possible.

If the product is dispatched to us in unsuitable packaging, you will be charged the cost for returning it to you in new packaging.

The forms can be downloaded online from www.martinchrist.de  $\rightarrow$  [Service]  $\rightarrow$  [Overhaul, repair and leak testing].



# 9 Disposal

# 9.1 Disposal of the freeze-dryer

Martin Christ Gefriertrocknungsanlagen GmbH is a registered manufacturer of electric and electronic devices that are solely intended for commercial use.

· Comply with all local rules and regulations.

# 9.2 Disposal of the packaging

- Dispose of the packaging, after having separated the individual materials.
- · Comply with all local rules and regulations.



# 10 Technical data

Manufacturer:	Martin Christ Gefriertrocknungsanlagen GmbH An der Unteren Söse 50 37520 Osterode (Germany)						
Type:	Epsilon 1-4 LSCplus	Epsilon 2-4 LSCplus					
Part number:	111141	111144					
Performance data	Epsilon 1-4 LSCplus	Epsilon 2-4 LSCplus					
<u>lce condenser chamber</u> - Dimensions (W x H x D): - Volume:	300 mm x 320 mm x 432 mm approx. 41 l	300 mm x 320 mm x 432 mm approx. 41 l					
Ice condenser - Capacity: - Performance: - Temperature:	max. 4 kg max. 3,0 kg / 24 h approx55°C	max. 4 kg max. 3,0 kg / 24 h approx85°C					
Shelves  - Number of shelves: - Dimensions (W x D): - Max. shelf surface area: - Distance between shelves without sealing device: with standard option sealing device: - Shelf temperature:	1 270 mm x 400 mm 0,108 m <sup>2</sup> 172 mm 140 mm approx45°C to +60°C	1 270 mm x 400 mm 0,108 m <sup>2</sup> 172 mm 140 mm approx70°C to +60°C					
Connection requirements	Epsilon 1-4 LSCplus	Epsilon 2-4 LSCplus					
Electrical connection:	1 x 230 V / 50 Hz (other supply data on request)	1 x 230 V / 50 Hz (other supply data on request)					
Protection class:	I	I					
IP-Code according to DIN 60529:	20	20					
Nominal power:	1.0 kVA	2.0 kVA					
Nominal current:	4.5 A	9.0 A					
Vacuum pump connection:	230 V, 50/60 Hz, 9.5 A max.	230 V, 50/60 Hz, 5.5 A max.					
Physical data (without vacuum pump)	Epsilon 1-4 LSCplus	Epsilon 2-4 LSCplus					
Dimensions  Basic unit - Height: - Width: - Depth:	520 mm 780 mm 598 mm incl. vacuum connection	520 mm 780 mm 598 mm incl. vacuum connection					
Weight (without vacuum pump):	approx. 110 kg	approx. 140 kg					
Noise level according to DIN 45635:	dB(A)	51 dB(A)					
EMC according to EN 55011:	Class B	Class B					
Heat emission:	min. 620 W max. 1,100 W	min. 1,100 W max. 1,600 W					



#### 10 Technical data

Regrigerant data	Epsilon 1-4 LSCplus	Epsilon 2-4 LSCplus
Refrigerant: - Global warming potential (GWP): - Filling quantity: - Max. permissible pressure: - CO <sub>2</sub> equivalent:	R1270 3 62 g 25 bar < 0,01 t	R1270 3 64 g 25 bar < 0,01 t
Refrigerant: - Global warming potential (GWP): - Filling quantity: - Max. permissible pressure: - CO <sub>2</sub> equivalent:	R170 3 6 g 25 bar < 0,01 t	R170 3 60 g 25 bar < 0,01 t

Equipment connections	Epsilon 1-4 LSCplus	Epsilon 2-4 LSCplus
Aeration:	Hose nozzle DN6 (outside diameter 10 mm max) max. +0.2 bar	Hose nozzle DN6 (outside diameter 10 mm max) max. +0.2 bar
Vacuum connection:	Small flange connection DN25KF (ISO 28403, DIN 2861)	Small flange connection DN25KF (ISO 28403, DIN 2861)
Mains input:	CEE 7/4 plug (type F)	CEE 7/4 plug (type F)
Data interface (LAN):	RJ45	RJ45

#### 10.1 Ambient conditions

- Use in closed spaces
- Altitudes up to 2,000 m
- Ambient temperature between +5°C and +25°C
- Maximum relative humidity of 80%
- Mains voltage fluctuations of up to ± 10% of the rated voltage

### 10.2 Technical documentation

The technical documentation of this freeze-dryer (e.g. circuit diagram, cooling system) and the safety data sheets of the manufacturers (e.g. for refrigerant) is not attached to this operating manual.

You can order these documents from our service department.



# 11 Appendix

# 11.1 Mathematical relations

The automatic processes in the "Programmer module" menu (see chapter 6.6.3 - " Freeze-drying with the PGMplus programmer module ") are based on the following considerations:

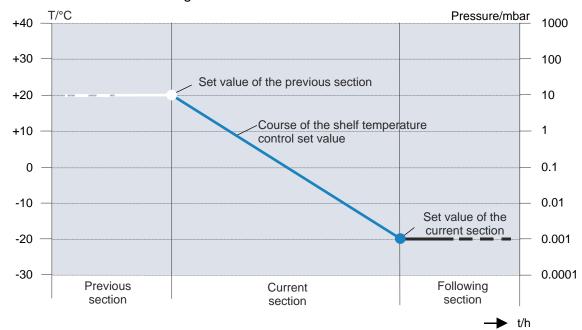


Fig. 78: Graphical representation of the course of the control set value

# Calculation of the control set value and of the gradient for the temperature:

$$gradient = \frac{set\ value\ of\ current\ section - set\ value\ of\ previous\ section}{section\ time\ of\ current\ section} \quad \ [°C/min]$$

 $control\ set\ value = set\ value\ of\ previous\ section + elapsed\ section\ time\cdot\ gradient\ [^{\circ}C]$ 

Example:	Section	Set values		
		Section time [h:min]	Temperature [°C]	
	Preceding		30	
	Current	1:00	60	

$$gradient = \frac{60 \text{ °C} - 30 \text{ °C}}{60 \text{ min}} = \frac{30 \text{ °C}}{60 \text{ min}} = 0.5 \text{ °C/min}$$

After an elapsed section time of 30 minutes, for example, the control set value for the temperature is:

Control set 
$$value_{(t=30 \text{min})} = 30 \text{°} C + 30 \text{min} \cdot 0.5 \text{°} C / \text{min} = 45 \text{°} C$$

#### Calculation of the control set value for the vacuum:

$$control\ set\ value = 10 \\ \begin{array}{c} LOG10(set\ value\ prev.\ sect.) + \left(\frac{LOG10(set\ value\ current sect. - LOG10(set\ value\ prev.\ sect.)}{section time\ of\ current\ section}\right) \\ elapsed\ section time\ of\ current\ section \\ [mbar] \\ [mbar] \end{array}$$

# 11 Appendix





# 11.2 EC declaration of conformity in accordance with the EC Machinery Directive



### **EC – DECLARATION OF CONFORMITY**

in accordance with the EC Machinery Directive 2006/42/EC, annex II, part 1, section A

The product named hereinafter was developed, designed, and manufactured in compliance with the relevant, fundamental safety and health requirements of the listed EC directives and standards.

In the event of modifications that were not authorised by us or if the product is used in a manner that is not in line with the intended purpose, this declaration will be rendered void.

Product name:	Freeze-dryer		
Product type:	Epsilon 1-4 LSCplus, Epsilon 2-4 LSCplus		
Order number:	111141, 111144		
Directives:	2006/42/EG Machinery Directive 2014/35/EU Low Voltage Directive 2014/30/EU EMC Directive 2014/68/EU Pressure Equipment Directive 2011/65/EU RoHS Directive		
- if the unit is equipped with WTMplus:	2014/53/EU Radio Equipment Directive		
Underlying standards:	DIN EN 378-1:2021-06 DIN EN 378-2:2018-04 DIN EN 378-3:2020-12 DIN EN 378-4:2019-12 DIN EN 61010-1:2020-03 DIN EN 60204-1:2019-06 DIN EN 61000-6-2:2019-11 DIN EN 61000-6-4:2020-09		
- if the unit is equipped with WTMplus:	EN 301489-1:2012-04 EN 301489-3:2013-12 EN 300330-1:2015-08 EN 300330-2:2015-08		

#### Martin Christ Gefriertrocknungsanlagen GmbH

An der Unteren Söse 50 Authorised representative 37520 Osterode for CE matters:

Germany S. Krippendorff

Osterode, 13/07/2022

F. Harms, Management

CE\_MaschRL\_Epsilon\_1-4\_2-4\_LSCplus\_Standard\_2-0\_2022-07-13\_en.docx

Page 1 / 1

# 11 Appendix





# 11.3 UKCA declaration of conformity



#### **UKCA – DECLARATION OF CONFORMITY**

The product named hereinafter was developed, designed, and manufactured in compliance with the relevant, fundamental safety and health requirements of the listed directives and standards. In the event of modifications that were not authorised by us or if the product is used in a manner that is not in line with the intended purpose, this declaration will be rendered void.

Product name:	Freeze-dryer
Product type:	Epsilon 1-4 LSCplus, Epsilon 2-4 LSCplus
Order number:	111141, 111144
Manufacturer:	Martin Christ Gefriertrocknungsanlagen GmbH An der Unteren Söse 50 37520 Osterode am Harz Germany
Directives:	Supply of Machinery (Safety) Regulations 2008 Electrical Equipment (Safety) Regulations 2016 Electromagnetic Compatibility Regulations 2016 Restriction of the Use of Certain Hazardous Substances in Electrical and Electronic Equipment Regulations 2012
Normes:	DIN EN 378-1:2021-06 DIN EN 378-2:2018-04 DIN EN 378-3:2020-12 DIN EN 61010-1:2020-03 DIN EN IEC 61000-6-2:2019-11 DIN EN IEC 61000-6-3:2022-06 DIN EN 55011:2022-05

UK Authorised Representative:



Osterode, 13/12/2022

Dr. F. Harms, Management

UKCA\_Epsilon\_1-4\_2-4\_LSCplus\_Standard\_2-0\_2022-12-13\_en.doc

Page 1 /

# 11 Appendix





# 11.4 EC declaration of conformity in accordance with the Pressure Equipment Directive



#### EC - DECLARATION OF CONFORMITY

in accordance with the EC Pressure Equipment Directive 2014/68/EU

The refrigeration units in freeze-dryers which are listed hereinafter were developed, designed, and manufactured in accordance with the relevant, fundamental safety and health requirements of the listed EC directives and standards.

In the event of modifications that were not authorised by us or if the product is used in a manner that is not in line with the intended purpose, this declaration will be rendered void.

Product name:	Refrigeration unit in a freeze-dryer	
Relevant unit types:	All laboratory systems of the following types: Alpha, Beta, Gamma, Delta Pilot systems of the following types: Epsilon 1-4,Epsilon 2-4 Epsilon 2-6D, Epsilon 2-10D	
Max. permissible pressure: Max. permissible temperature:	25 bar 120°C	
Directives:	2014/68/EU Pressure Equipment Directive	
Underlying standards:	AD 2000 EN 378	
Applied conformity assessment procedures:	Module A Category I	

#### Martin Christ Gefriertrocknungsanlagen GmbH

An der Unteren Söse 50 37520 Osterode Germany

Authorised representative for CE matters: S. Krippendorff

Osterode, March 8, 2022

F. Harms, Management

CE\_DruckGRL\_Labor+Pilot\_2022-03-08\_en.doc

Page 1 / 1

# 11 Appendix





# 11.5 Table of the sublimation pressure curve

°C	= mbar						
0	6,110	-20	1,030	-40	0,120	-60	0,011
-1	5,620	-21	0,940	-41	0,110	-61	0,009
-2	5,1770	-22	0,850	-42	0,100	-62	0,008
-3	4,760	-23	0,770	-43	0,090	-63	0,007
-4	4,370	-24	0,700	-44	0,080	-64	0,006
-5	4,020	-25	0,630	-45	0,070	-65	0,0054
-6	3,690	-26	0,570	-46	0,060	-66	0,0047
-7	3,390	-27	0,520	-47	0,055	-67	0,0041
-8	3,010	-28	0,470	-48	0,050	-68	0,0035
-9	2,840	-29	0,4202	-49	0,045	-69	0,0030
-10	2,560	-30	0,370	,50	0,040	-70	0,0026
-11	2,380	-31	0,340	-51	0,035	-71	0,0023
-12	2,170	-32	0,310	-52	0,030	-72	0,0019
-13	1,980	-33	0,280	-53	0,025	-73	0,0017
-14	1,810	-34	0,250	-54	0,024	-74	0,0014
-15	1,650	-35	0,220	-55	0,021	-75	0,0012
-16	1,510	-36	0,200	-56	0,018	-76	0,0010
-17	1,370	-37	0,180	-57	0,016	-77	
-18	1,250	-38	0,160	-58	0,014	-78	
-19	1,140	-39	0,140	-59	0,012	-79	

# 11 Appendix





# 12 Glossary

#### Aeration, stoppering, storage

"Aeration, stopperting, storage" means automated sealing of the product vials with previously inserted rubber stoppers under partial vacuum and subsequent storage on the shelves at defined conditions as an integral part of a freeze-drying program. This is why this option can only be used in combination with a programmer module and if the freeze-dryer is equipped with an automatic aeration valve and a hydraulic shelf movement system.

#### **Comparative pressure measurement**

During the → *sublimation*, i.e. when the concentration of water vapour molecules is rather high in the atmosphere, the value that is provided by the gas-type dependent vacuum sensor of the "Pirani" type (e.g. Thyracont VCP 63) deviates from the value that is provided by a capacitive vacuum sensor (e.g. Pfeiffer CMR363). When the proportion of water vapour molecules decreases towards the end of the main drying phase, the two sensors fall increasingly in line with one another.

The comparative pressure measurement is often used as a criterion for the automatic switching from the main drying phase to the final drying phase as well as for identifying the end of the process.

#### **Desorption**

Desorption (from Latin de-sorbere, sorbere = sup up, suck in) describes a phenomenon whereby molecules are released from the surface of a solid. In order to be able to desorb, the particle must have, or be provided with, a sufficient amount of energy in order to overcome the binding energy.

#### **Double-chamber method**

Freezing and drying of the product on several temperature controlled shelves inside a separated drying chamber is referred to as a double-chamber system. The advantage compared to the  $\rightarrow$  *single-chamber method* is the considerably higher product capacity. In addition, the product chamber can be isolated from the ice condenser chamber by an intermediate valve in order to perform a so-called  $\rightarrow$  *pressure increase test* for determining the end of the drying process.

#### **Eutectic point**

The eutectic point is the point at which a homogenous mixture (e.g. an eutectic alloy) passes directly from the liquid to the solid phase without the formation of a crystal mixture that consists of different phases.

#### Leakage test

The leakage test enables the chamber of the freeze-dryer to be tested for tightness in view of any gaseous or liquid media. Since absolutely tight components simply do not exist, a leak rate is determined. The parameters for the leakage test have been developed by Martin Christ Gefrier-trocknungsanlagen GmbH specifically for freeze-dryers. In a first step, these parameters (vacuum, ice condenser temperature) must be reached. It is not until the conditions are fulfilled that the pressure control valve closes. Then, the actual leakage test is performed in a second step. The leak rate that is calculated after the end of the test provides information concerning the tightness of the system.



#### Pressure increase test

The pressure increase test can only be carried out with  $\rightarrow$  double-chamber method. During the pressure increase test, the intermediate valve prevents the flow of steam from the drying chamber to the ice condenser so that the water vapour of the  $\rightarrow$  sublimation cannot flow off. The result is a more or less distinct pressure increase that is measured in the product chamber. When the product has been completely dried, the vacuum does not decrease at all or only to a slight extent.

The pressure increase test is often used as a criterion for the automatic switching from the main drying phase to the final drying phase as well as for identifying the end of the process.

#### Reference designator

During the service life of industrial systems, a standardised reference designation system is required for the planning, design, realisation, maintenance, and disassembly stages in order to be able at all times to identify every single component within the system in an unambiguous manner. The reference designators are affixed to the components and entered into the technical documentation (e.g. circuit diagrams).

#### Safety pressure

Since the vacuum has a dominating influence on the product temperature, Martin Christ Gefriertrocknungsanlagen GmbH has integrated a so-called safety pressure feature into the freeze-dryers in order to ensure the protection of the product. If the pressure inside the drying chamber increases too strongly so that it exceeds the safety limit, the energy supply of the shelves will be interrupted and the  $\rightarrow$  *sublimation* process slows down. This prevents the product from melting.

The safety pressure value that is entered should correspond to a temperature value that is 5°C below the melting point of the product on the vapour pressure curve above ice.

#### Single-chamber method

At the single-chamber method, the freezing as well as the subsequent drying of the product are both performed on several temperature controlled shelves inside the ice condenser chamber.

#### **Sublimation**

Sublimation (from Latin "sublimis" = high up in the air, raised), is a thermodynamic process of the direct transition of a substance from the solid phase to the gas phase.



A	
Access protection77	2006/42/EC
Accessories 39, 114, 122	Chamber, cleaning and care
Accident prevention25, 28	Changing of operating supplies
Accident prevention regulations25	Chemical reactions
Accidents	Circuit diagram
Acids12, 38	Cleaning
Acids (hazards)32	Cleaning agents
Actual values of the current process 58	Cleaning the accessories
Additions38	Cleaning the accessories114  Cleaning the freeze-dryer114
Administration75	Click on touch
Aeration46	CO <sub>2</sub> equivalent
Aeration (connection)136	Comparative pressure measurement
Aeration medium, preselection 72, 106	97, 105, 147
Aeration valve, cleaning and care117	Compatibility test25, 26
Aeration valve, malfunction111	Compliance with the EC health and safety
Aeration, stoppering, storage 98, 106, 147	directives25
Ambient conditions136	Condensate, contaminated (hazards) 33
Ambient temperature 45, 136	Conditions for switching to the next section 91
Apparent power17	Configuration of sensors79
Areas of responsibility25	Connection
Automatic aeration, stoppering, storage 106	Connection (hazards)29, 45
Azides12	Connection requirements135
Azides (hazards)32	Contaminated condensate (hazards)33
В	Contaminated defrosting water (hazards) 33
Beeper76	Control switch36
Behaviour of the pressure control valve in the	Control system type86
case of insufficient ice condenser cooling	Controlled Nucleation LyoCoN104
77	Conversions38
Burns 37	Cooling system136
Button "Set values: view/edit"58	Copying a program102
Button "Standard unit test" 64	Copyright13
Button "Stop" 69	Corrosion114, 122
C	Cost estimate133
Calculation of the control set value and of the	Cracks 122
gradient for the temperature	Creating a blank program93
Calculation of the control set value for the	Creating a program93
vacuum137	Customer-provided fuses46
Capacity test -30°C66	D
Capacity test -50°C67	Damage to the materials of construction 114



Danger of infection due to exhaust air 49	Editing a program101
Danger of poisoning due to exhaust air 49	Electrical connection135
Dangerous materials123	Electrical system (maintenance) 118
Data interface (LAN) 136	Electricity (hazards)30, 118
Date/Time75	Emergency37
Declaration of conformity (Machinery	End of drying and aeration22
Directive) 13, 139	Entering set values in the manual mode 87
Declaration of conformity (Pressure	Environmental protection28
Equipment Directive)	Equipment connections136
Declaration of decontamination	Equipotential bonding screw36
Decontamination agents123	Error correction108
Defrosting	Eutectic point147
Defrosting water, contaminated (hazards) 33	Exhaust air (hazards)34, 120
Defrosting with hot gas	Exhaust filter48
Deleting a program	Exhaust filter (oil mist separator) and vacuum
delta p pressure increase test (option) 91	pump (oil-sealed)47
deltaT comparative91	Exhaust gases (hazards) 33, 34, 47, 120
deltaT product	Exhaust gases of the vacuum pump 49
deltaT shelf91	Explanation of symbols13
Desorption	Explanation of the symbols and notes24
Details	Explosive substances32
Process and equipment messages 63	External data storage device58
Details concerning the software version 86	F
Device options78	Failure memory83
Dialog box "New program"70	Fast freezing (improved cooling rate) 104
Dialog box "Operating mode: select/start" 64	Filling quantity (refrigerant)
Dialog box "Process and equipment	Film "Radiation Shield"55, 116
messages"	Film on the loading door (cleaning) 116
Dialog box "Schematic system diagram" 61	Final drying22
Dialog box "Tools"	Fire
Dimensions	Fire prevention
Direct hazard to the life and health24	Form for the return of defective parts 133
Disinfectants	Freeze-dryer type86
Disinfection of the drying chamber and accessories	Freeze-dryer, cleaning and care115
Displayed vacuum value is not correct 109	Freeze-drying of acid-containing products 12
Disposal of the freeze-dryer 134	Freeze-drying of azide-containing products 12
Disposal of the packaging	Freeze-drying of solvent-containing products
Door latch	
Double-chamber method147	Freeze-drying phases20
	Freeze-drying process20
E	Freeze-drying with the PGMplus programmer
Earth conductor check36	module89
EC declaration of conformity (Machinery	Freezing21
Directive)	Functional and operating elements14
EC declaration of conformity (Pressure Equipment Directive)	Further applicable documents9





G	I
Gas injection with a proportional valve73, 106	Ice condenser 135
General conditions12	Ice condenser temperature91
General information on freeze-drying18	Importance of the operating manual9
General malfunctions108	Important information24
General tasks (maintenance) 114	Improved cooling rate (fast freezing) 104
Global warming potential (GWP)136	Inertisation74, 106
H	Infectious substances123
Handling hazardous materials39	Informal safety notes28
Hazard warnings	Initial start-up53
Hazardous materials, handling39	Initial start-up (hazards)29, 53
Hazards37	Injuries37
	Inspection by the manufacturer132
Hazards (acids)32 Hazards (azides)32	Installation of accessories53
•	Installation site45
Hazards (connection)	Instruction25
Hazards (contaminated condensate)33	Insufficient ice condenser or shelf
Hazards (contaminated defrosting water)33	temperature109
Hazards (electricity)	Insufficient ice condenser temperature 112
Hazards (exhaust air)34, 120	Insufficient vacuum 108, 110
Hazards (general, transport to commissioning)28	Intended use9
	IP-Code135
Hazards (general, transport)	L
Hazards (initial start-up)29, 53	
Hazards (loading door)35	LAN process recording (RJ45) 105
Hazards (nitrogen)31	Language71
Hazards (noise)	Layout of the freeze-dryer14
Hazards (products, harmful)	Leakage in a rubber valve
Hazards (refrigeration system) 30, 121	Leakage in the media drain valve
Hazards (set-up)	Leakage test
Hazards (solvents)31	Loading a program102
Hazards (surfaces, cold)35	Loading door (film)116
Hazards (surfaces, hot)35, 115, 119, 120	Loading door (hazards)35
Hazards (transport)29, 42, 43	Loading door (operation)54
Hazards (vacuum pump exhaust gases)	LPCplus SCADA System105
33, 47	LSCplus control system56
Hazards (vacuum pump oil)	Lyes38
Health and safety25	LyoBalance weighing system61, 106
Health and safety rules and regulations and	LyoCam monitoring camera system 105
regulations for the prevention of accidents25, 27	LyoCoN Controlled Nucleation104
Heat emission135	LyoControl measuring system105
Heat exchanger118	LyoControl-Rx91
Hot-gas defrosting22	LyoLogplus data logging software105
Humidity136	M
130	Main drying21
	ivialit dryllig21



Main window "?"86	0
Main window "Manual"57	Oil mist separator48
Main window "Options"71	Oil mist separator (exhaust filter) and vacuum
Main window "Program"70	pump (oil-sealed)47
Mains voltage136	Operating elements14
Maintenance 38, 82, 85	Operating hours82
Maintenance (electrical system)118	Operating mode: select/start64
Maintenance (general tasks)114	Operating personnel25
Maintenance (refrigeration system) 121	Operating status58
Maintenance (vacuum sensor) 122	Operating voltage46
Maintenance (vacuum system) 119, 120	Operation38
Maintenance and service114	Operational safety122
Maintenance performed by the user 114	Operator (responsibility)25
Maintenance schedule (dry-running vacuum pump)128	Option: Aeration, stoppering, storage 98 Option: Comparative pressure measurement
Maintenance schedule (oil-sealed vacuum	·97, 105
pump)124	Option: Controlled Nucleation LyoCoN 104
Malfunction of the pressure control valve . 111	Option: Improved cooling rate (fast freezing)
Malfunctions108	104
Manual freeze-drying86	Option: LAN process recording (RJ45) 105
Manufacturer114, 123, 134, 135	Option: LPCplus SCADA System105
Manufacturer contact data86	Option: LyoBalance weighing system. 61, 106
Marking of the unit23	Option: LyoCam monitoring camera system
Materials of construction, damage 114	
Mathematical relations137	Option: LyoControl measuring system 105
Max. humidity136	Option: LyoLogplus data logging software 105
Maximum current for the vacuum pump48, 49	Option: Pressure increase test 60, 95, 104
Measures to be taken to ensure safe	Option: USB process recording 60, 106
operation38	Option: Weighing system98
Mode of operation18	Option: Wireless product temperature
Monitoring camera system LyoCam 105	measurement system WTMplus 104
N	Optional equipment104
Name plate17	Р
Network76	Packaging134
Network drive58	Part number 17, 135
New program70	Password input fails108
Nitrogen (hazards)31	Password operator/ maintenance/
No indication on the display 108	administrator78
Noise (hazards)34	Password timer runtime77
Noise level 135	Pathogenic substances115, 123
Noise measurement25	Performance data135
Nominal current	Performance test65
Nominal power	Physical data135
Nominal voltage17	Pilot and production systems, unit test 64
Notes on safety and hazards9	Potential hazard to the life and health 24
	Potentially hazardous situation24





Power failure109	Safety area39
Power supply46	Safety data sheets136
Preparation	Safety devices36
Preselection of the aeration medium 72, 106	Safety distance45
Pressure control valve50	Safety instructions
Pressure control valve, malfunction 111	Safety notes concerning set-up and
Pressure increase test 60, 95, 104, 148	connection28
Pressure marks122	Safety notes concerning the initial start-up. 28
Pressure measurement, comparative 105	Safety notes concerning the operation 30
Prevention of accidents9	Safety notes concerning the transport28
Process and equipment messages 62	Safety pressure148
Process and error messages112	Safety-conscious work25
Process data57	Schematic system diagram61
Product residues115	Sensor adjustment85
Product temperature measurement system	Serial number 17, 86, 113, 132
WTMplus104	Service132
Products containing acids12	Service contact113
Products containing azides12	Service life114
Products, harmful (hazards)31, 115	Service work132
Program list70	Set process values58
Program sections90	Set-up38
Program templates101	Set-up (hazards)29, 45
Protection class135	Set-up and connection45
Q	Shelf cooling test68
Qualified electrician28	Shelf mapping test68
	Signs of corrosion122
R	Silencer and vacuum pump (dry-running) 49
Radiation Shield film 55, 116	Single-chamber method148
Radioactive substances 115	Small flange connections110
Rated current17	Solvent-containing products11
Reference designator 61, 63, 82, 148	Solvents38
Refrigerant data 17, 136	Solvents (hazards)31
Refrigeration problems	Solvents114
Conditions at the location of use45	Special equipment104
Refrigeration system (hazards) 30, 121	Special equipment: Aeration, stoppering,
Refrigeration system (maintenance) 121	storage106
Remaining hazards40	Special equipment: Gas injection with a
Requirements concerning the personnel 27	proportional valve73, 106
Responsibility of the operator25	Special equipment: Inertisation 74, 106
Return of defective parts132	Special equipment: Preselection of the
Risk assessment25	aeration medium
Rubber valves52, 111	Specialised personnel 27
S	Specialist personnel
Safe operation38	Standard unit test
Safety and hazard notes28	Standards and regulations
23.21, 3.14 1142414 115100 11111111111111111111111111111	Status line58



Storage41	UV radiation 45, 114
Storage and transport41	V
Storage conditions41	Vacuum91
Stress-corrosion122	Vacuum connection
Sublimation148	Vacuum pump (dry-running) and silencer 49
Supply voltage46	Vacuum pump (oil-sealed) and exhaust filter
Surfaces, cold (hazards)35	(oil mist separator)47
Surfaces, hot (hazards)35, 115, 119, 120	Vacuum pump connection135
Switching the freeze-dryer OFF107	Vacuum pump exhaust gases49
Switching the freeze-dryer on53	Vacuum pump exhaust gases (hazards)
System properties76	33, 47
Т	Vacuum pump is not activated109
Table of the sublimation pressure curve 145	Vacuum pump oil (hazards) 34, 119
Technical data135	Vacuum pump oil change84
Technical documentation136	Vacuum pump warm-up92
Thermal stress 45, 114	Vacuum sensor51, 111
Tools59	Vacuum sensor (maintenance)122
Topping-up of operating supplies38	Vacuum system (maintenance) 119, 120
Touchpanel does not react108	Vapour pressure curve above ice59
Toxic substances115	Vapour pressure curve for ice and water 19
Training25	Ventilation45, 112
Transport41	Viewing or editing the set values88
Transport (hazards)29, 42, 43	W
Transport (hazards, general)42, 43	Warranty and liability12
Transport safety devices44	Weighing system98
Transport to commissioning (hazards,	Weighing system LyoBalance 61, 106
general)28	Weight 41, 135
Type 17, 135	Wireless product temperature measurement
U	system WTMplus104
Unit of measurement72	WTMplus configuration81
Unit test of pilot and production systems 64	WTMplus wireless product temperature
Unpacking the freeze-dryer42	measurement system104
USB process recording60, 106	Y
User interface56	Year of manufacture17